

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/14/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:41
INTERNAL STANDARD	VERIFIED	15:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:41
BLANK TEST	0.00	15:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:42
BLANK TEST	0.00	15:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:44
BLANK TEST	0.00	15:45

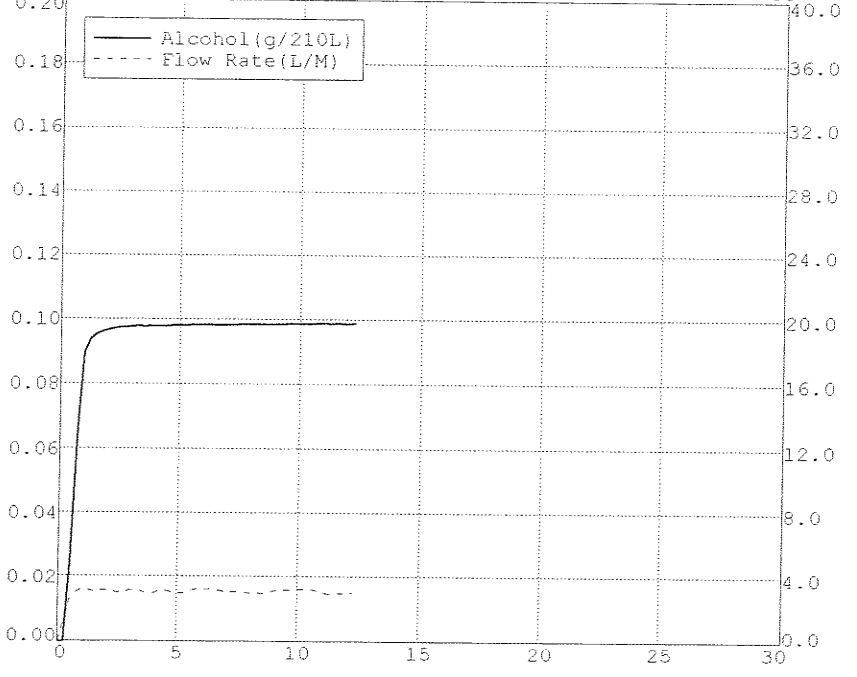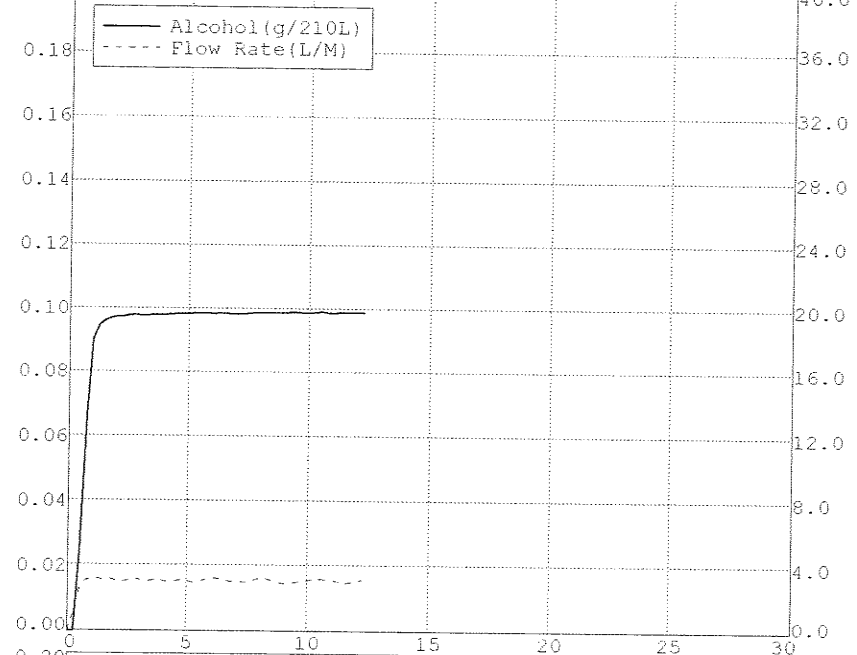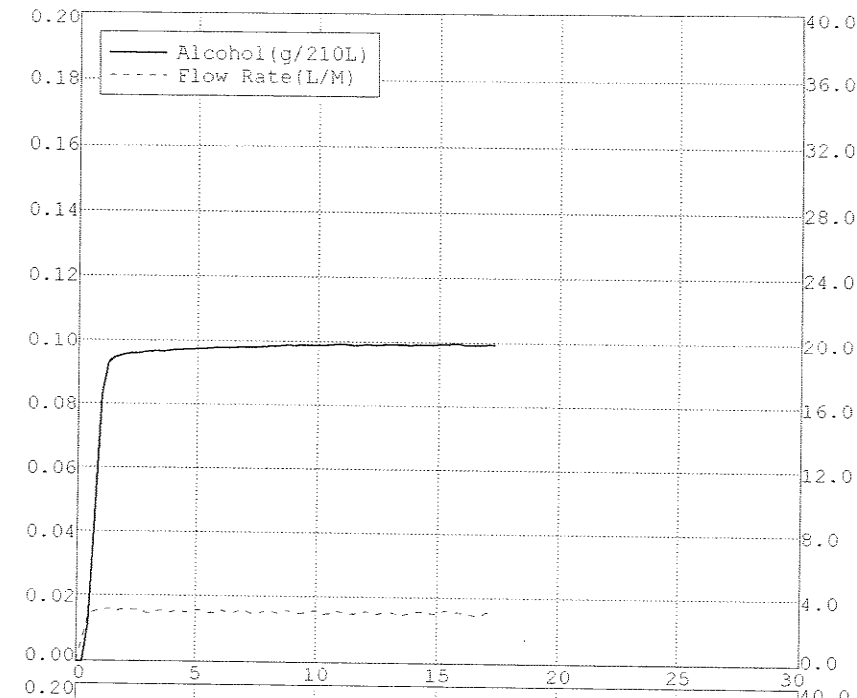

Charles B. Geisler #201