

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 02/22/2021

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:10
INTERNAL STANDARD	VERIFIED	10:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:10
BLANK TEST	0.00	10:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:12
BLANK TEST	0.00	10:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:13
BLANK TEST	0.00	10:14

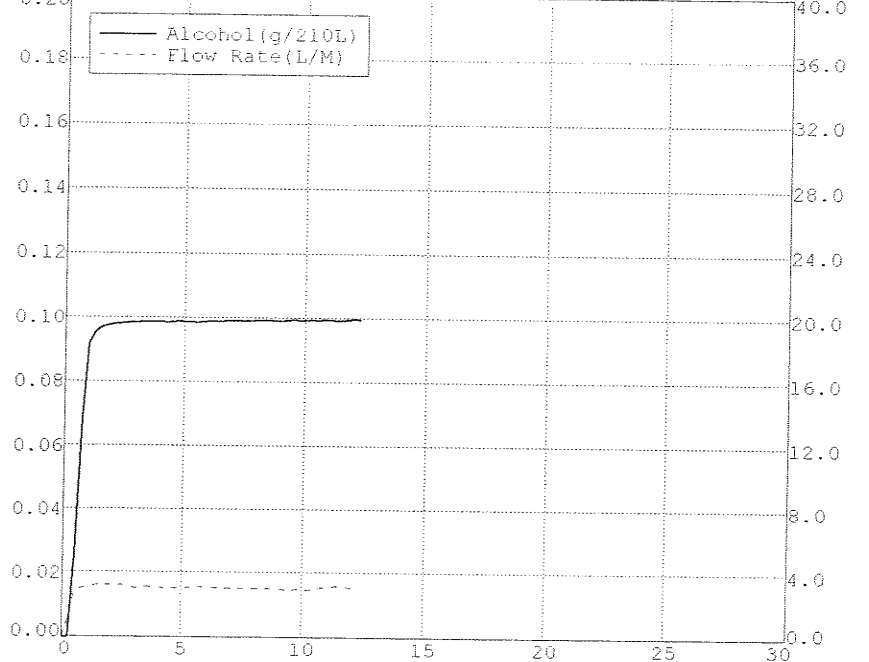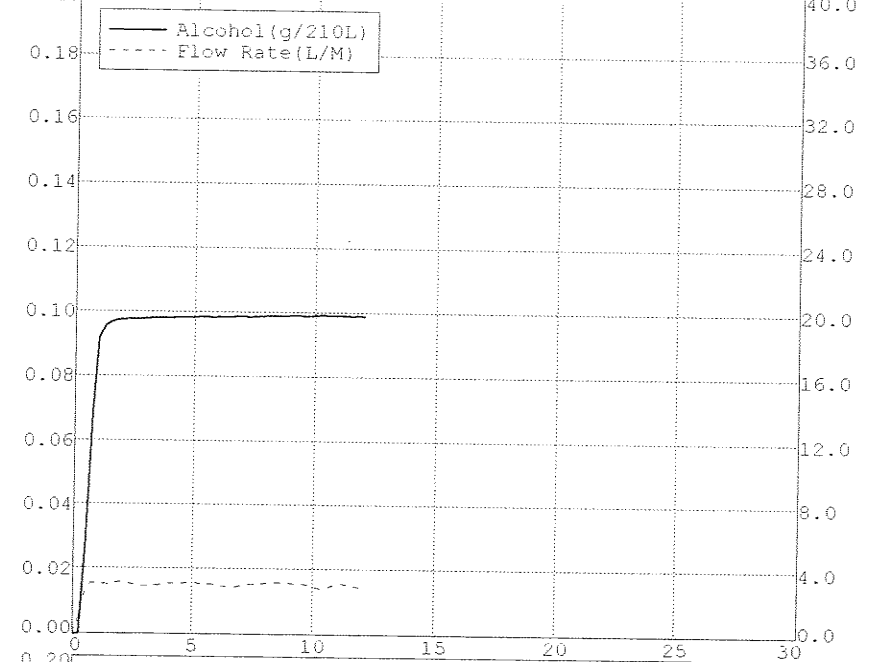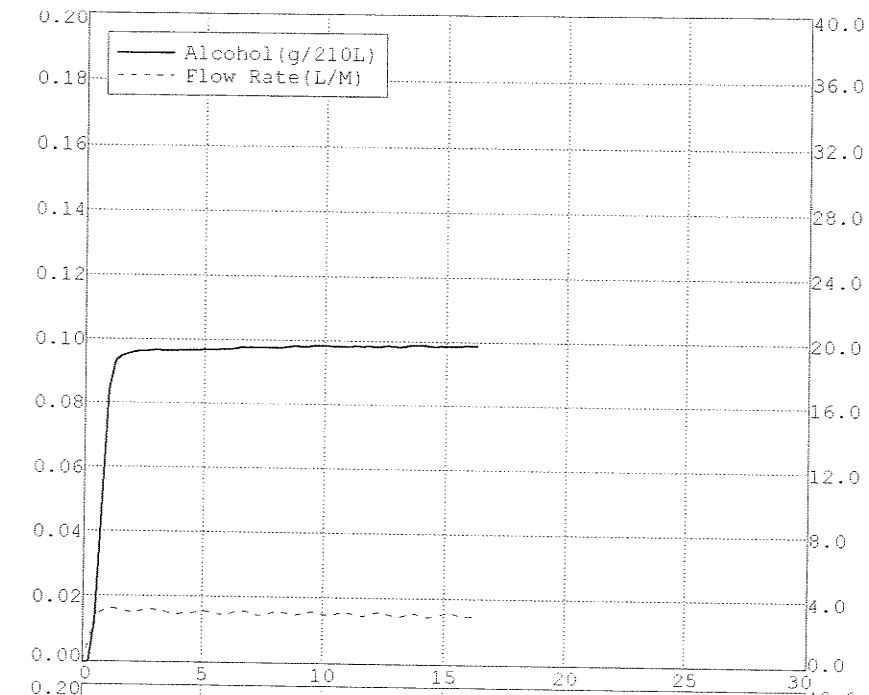

Handwritten signature and initials: J. P. ... #124