

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 03/08/2021

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:13
INTERNAL STANDARD	VERIFIED	15:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:13
BLANK TEST	0.00	15:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:14
BLANK TEST	0.00	15:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:15
BLANK TEST	0.00	15:16

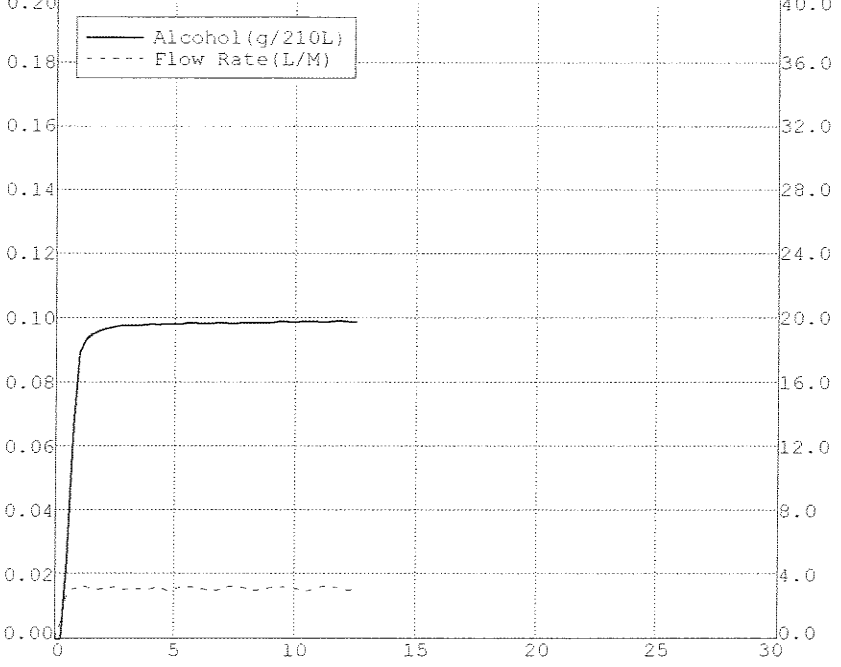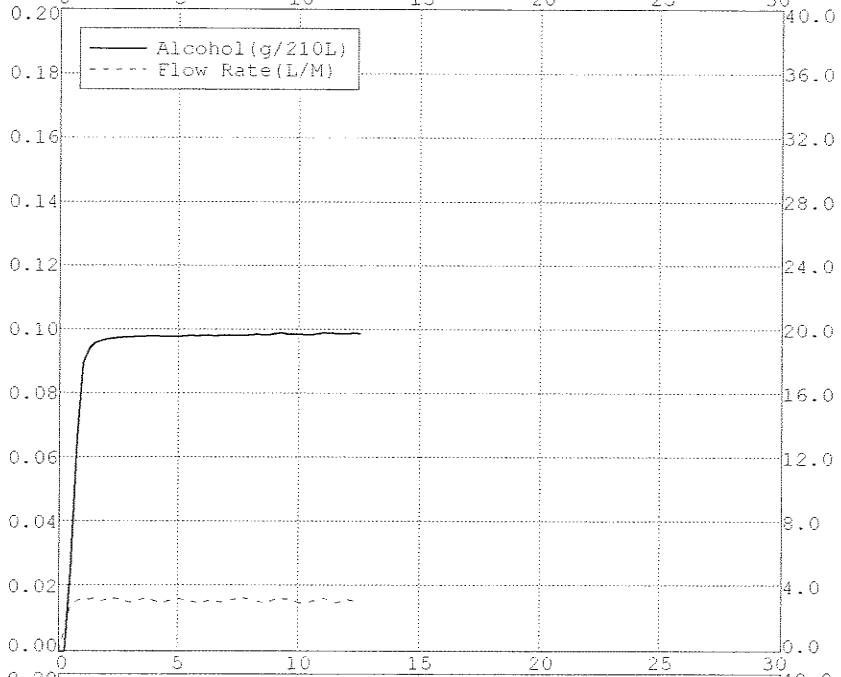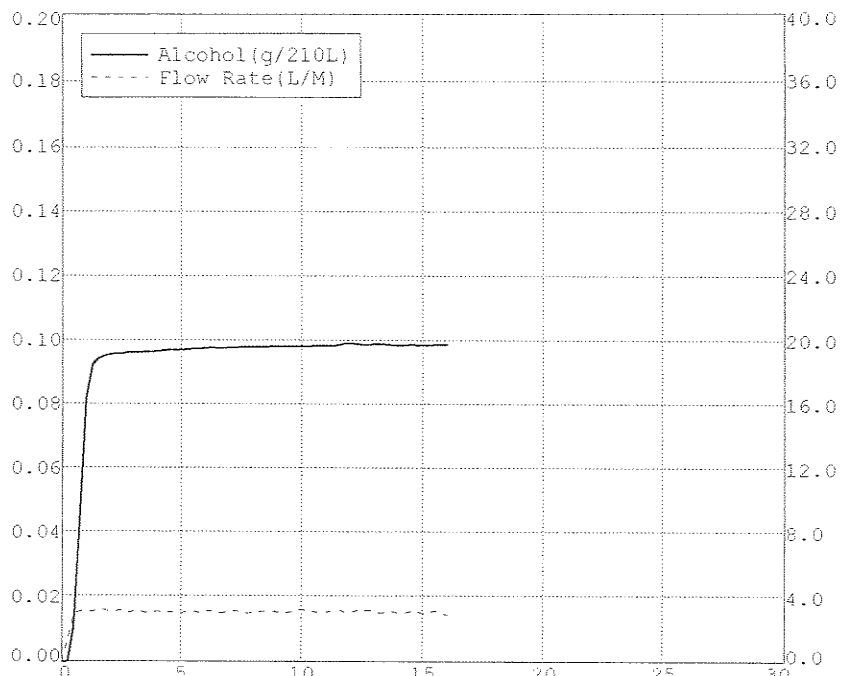

*Sgt. Charles B. Geisler #248*