

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 03/14/2021

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:26
INTERNAL STANDARD	VERIFIED	15:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:26
BLANK TEST	0.00	15:27
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:28
BLANK TEST	0.00	15:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:29
BLANK TEST	0.00	15:30

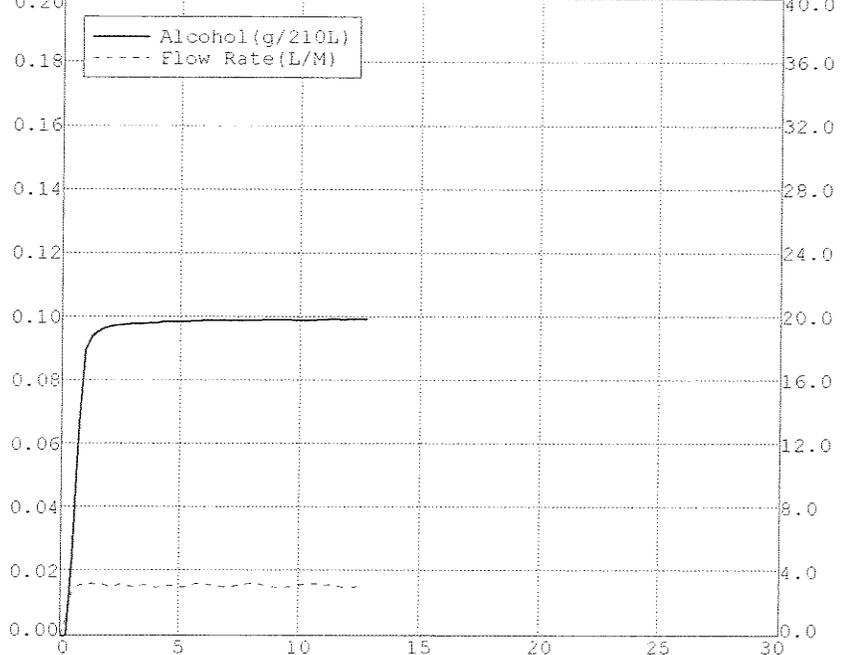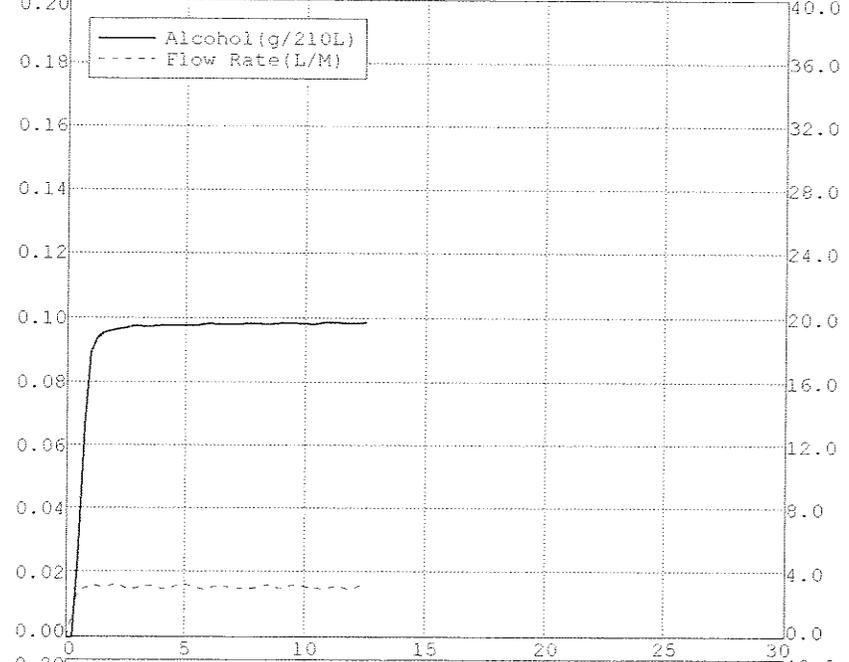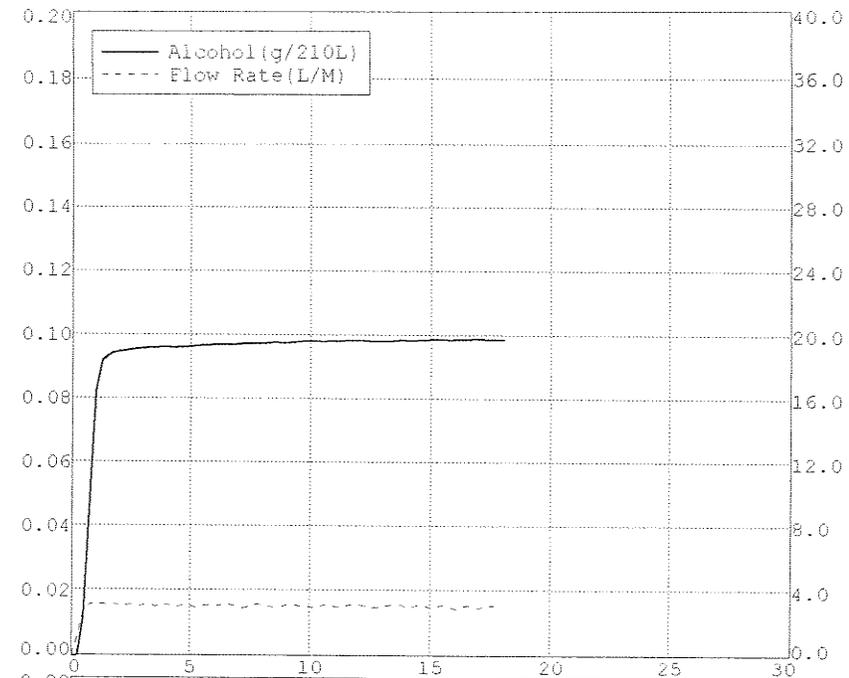

Sgt. C. B. Geisler