

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/22/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:15
INTERNAL STANDARD	VERIFIED	12:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:15
BLANK TEST	0.00	12:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:17
BLANK TEST	0.00	12:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:18
BLANK TEST	0.00	12:19

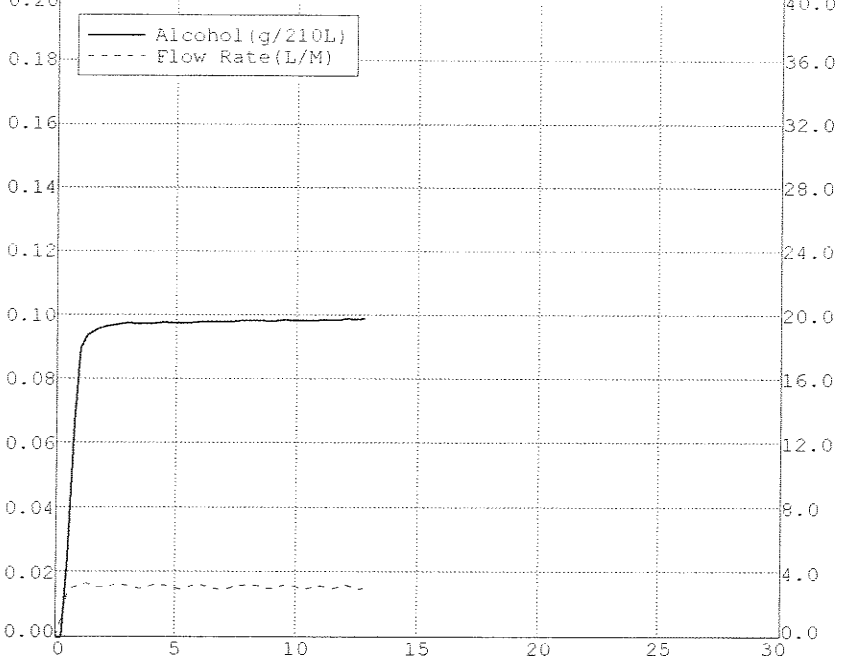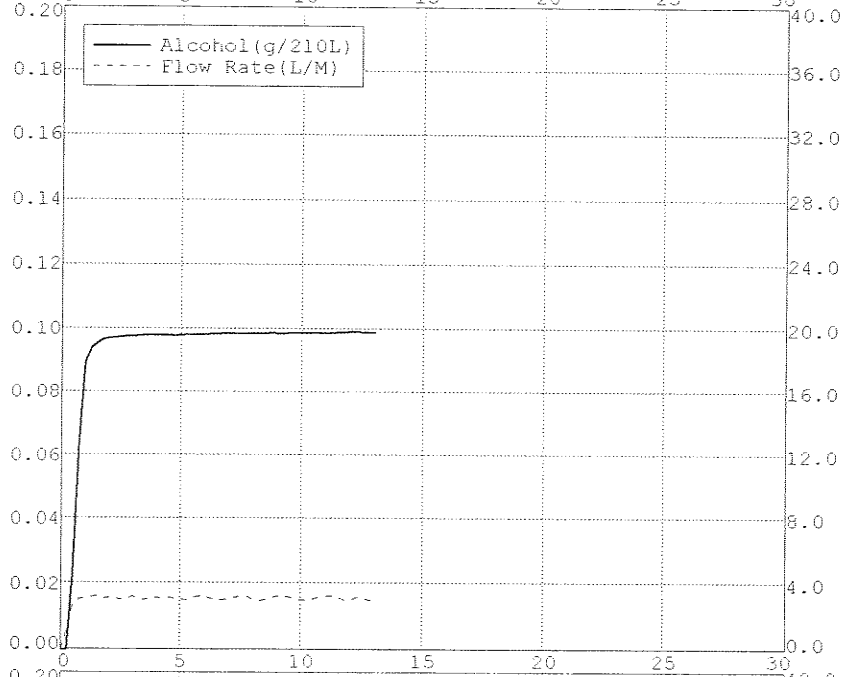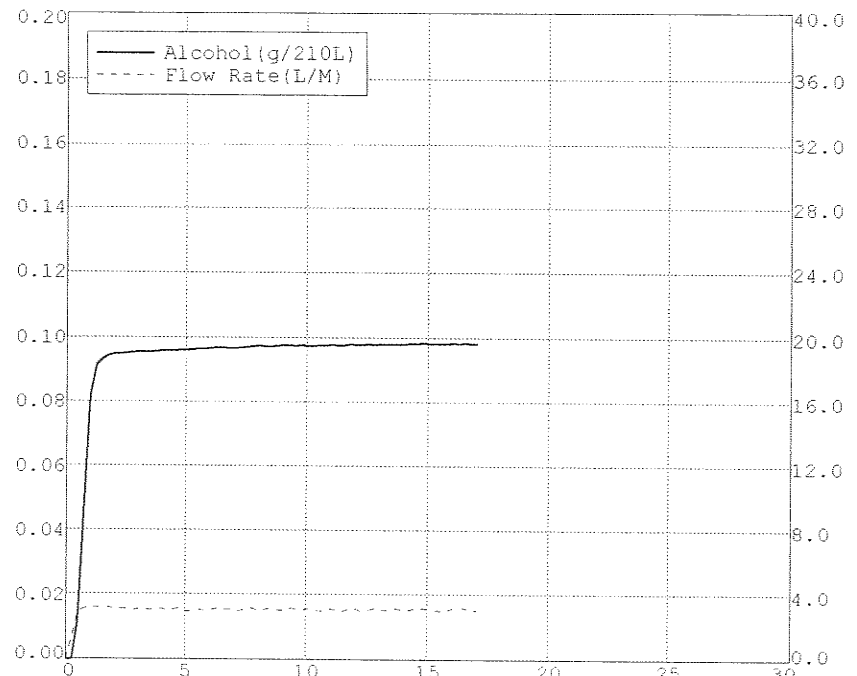

J. M. - 10 *[Signature]* #241