

SOLUTION CHANGE




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 03/31/2021

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:10
INTERNAL STANDARD	VERIFIED	16:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:10
BLANK TEST	0.00	16:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:11
BLANK TEST	0.00	16:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:13
BLANK TEST	0.00	16:13

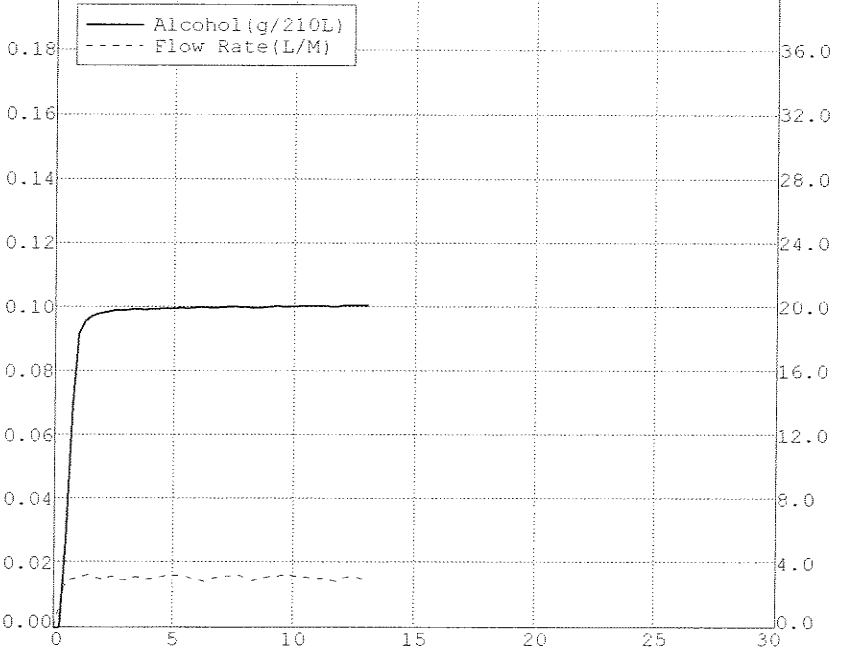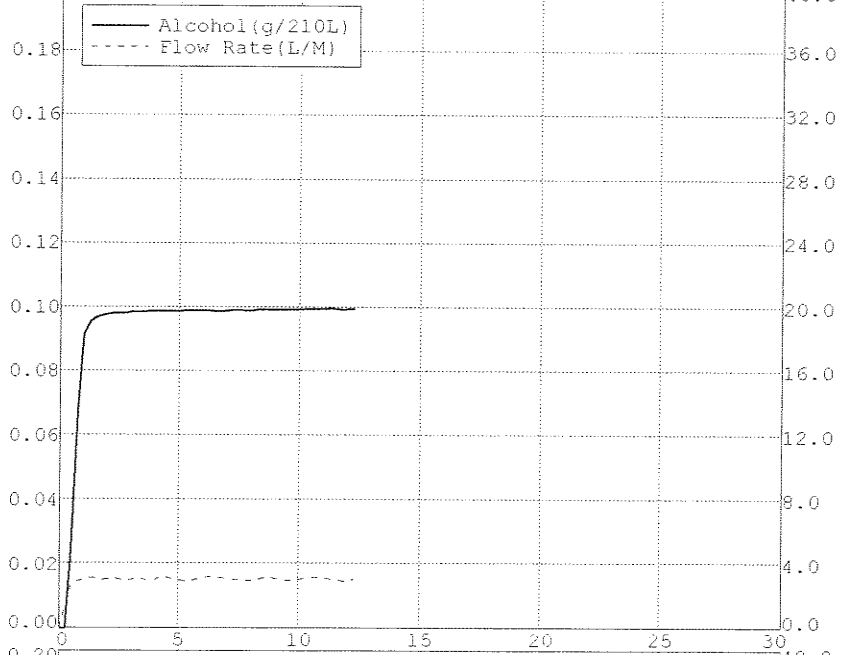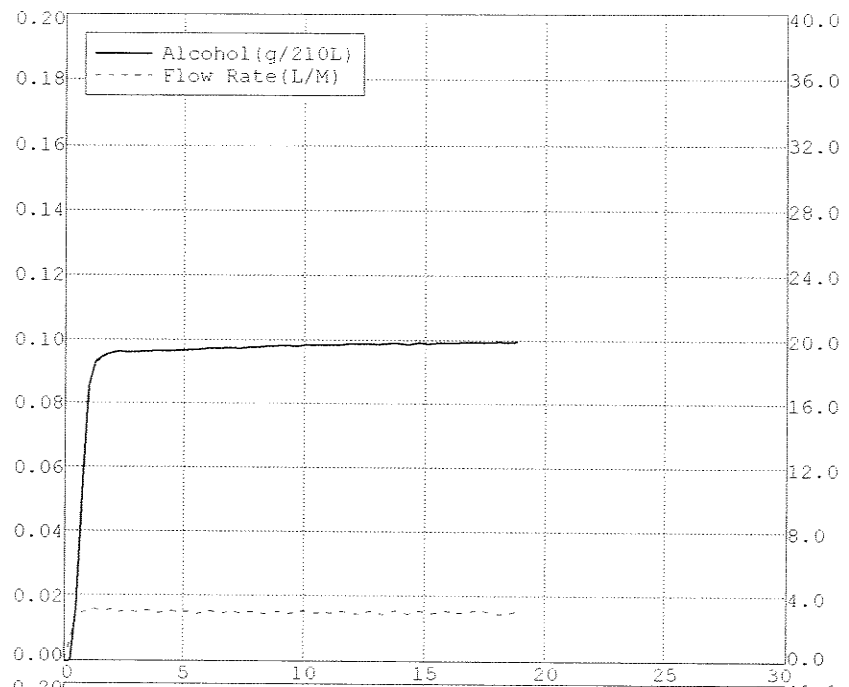

Handwritten signature: J. A. B. #24