

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/06/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:31
INTERNAL STANDARD	VERIFIED	15:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:31
BLANK TEST	0.00	15:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:32
BLANK TEST	0.00	15:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:34
BLANK TEST	0.00	15:35

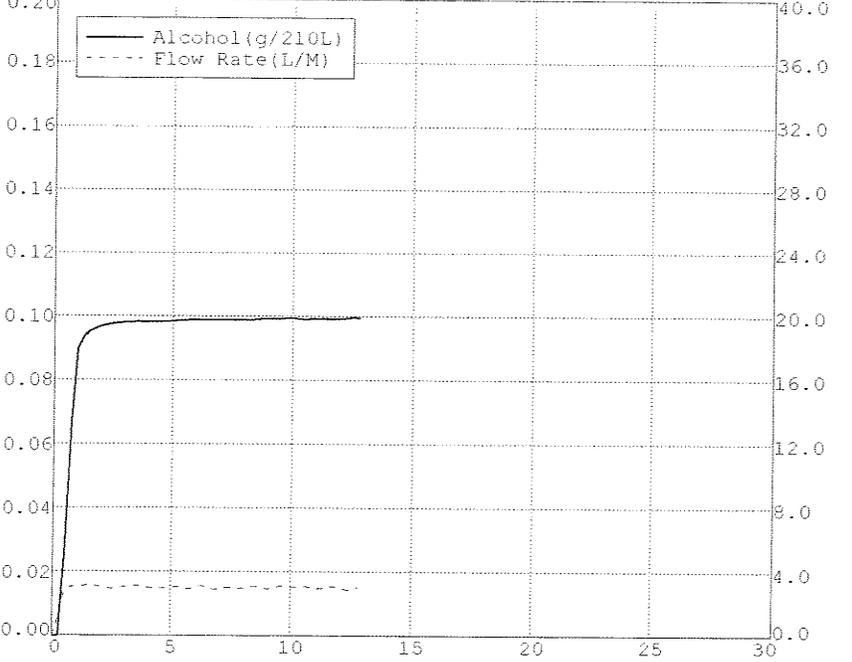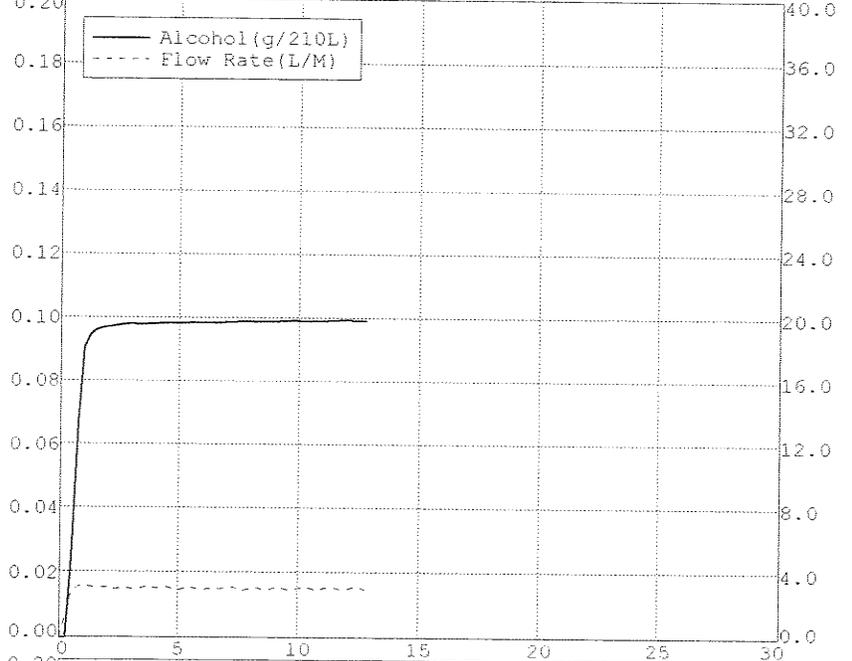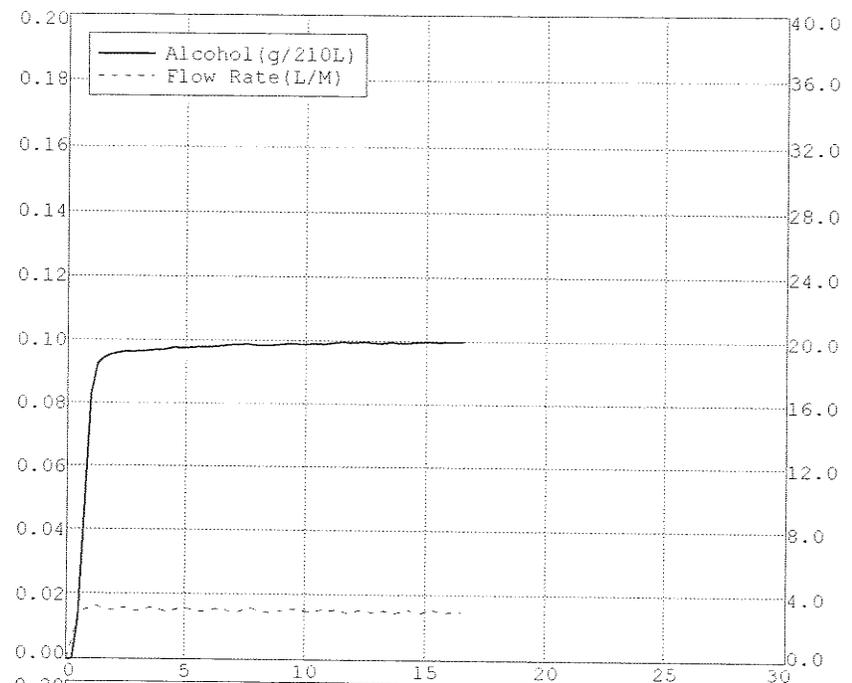

sgl *Chl-13* *[Signature]* *Hzw*