

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/11/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:50
INTERNAL STANDARD	VERIFIED	11:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:50
BLANK TEST	0.00	11:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:51
BLANK TEST	0.00	11:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:52
BLANK TEST	0.00	11:53

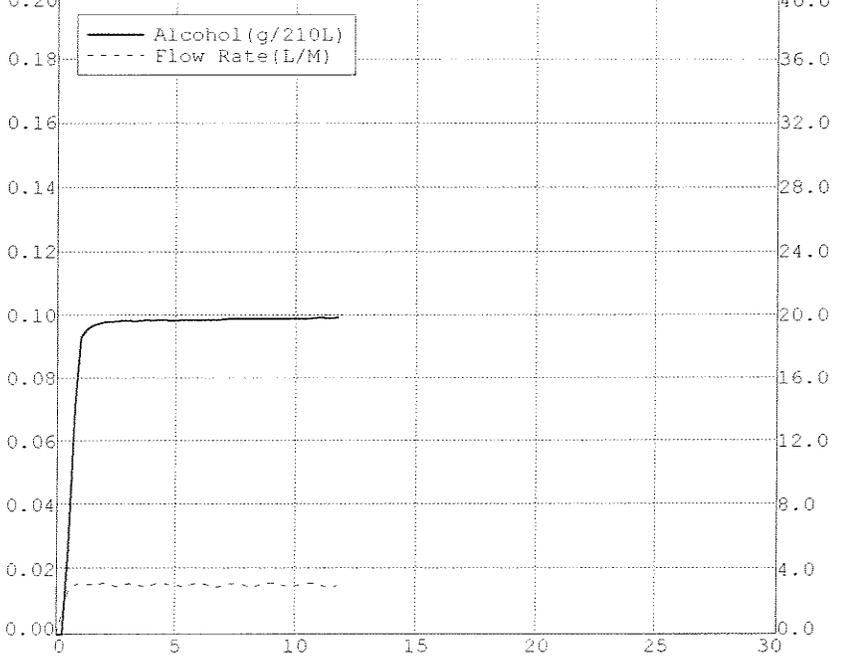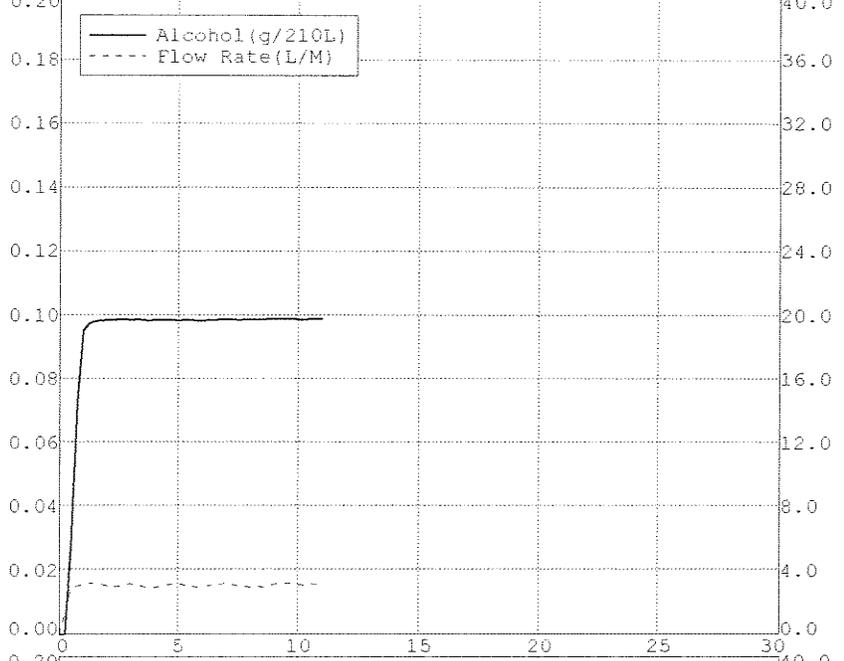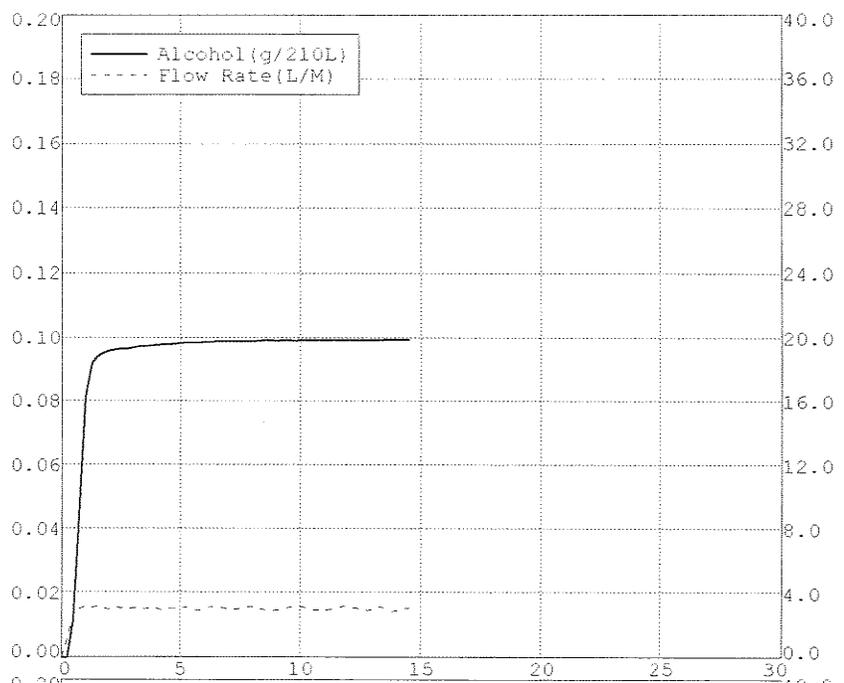

Handwritten signatures and initials:
J. C. B. [Signature] #248