

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 04/19/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:49
INTERNAL STANDARD	VERIFIED	14:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:50
BLANK TEST	0.00	14:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:51
BLANK TEST	0.00	14:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:52
BLANK TEST	0.00	14:53

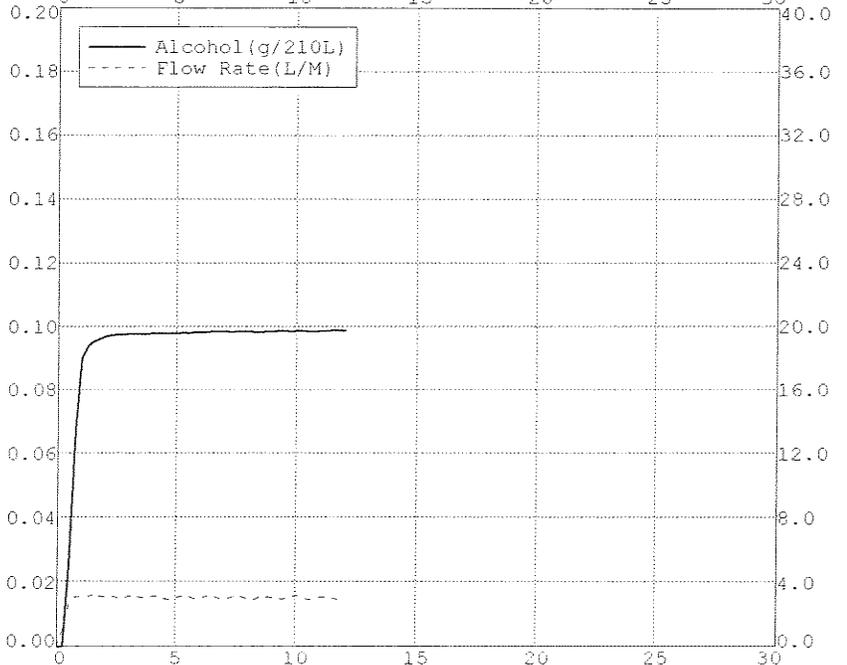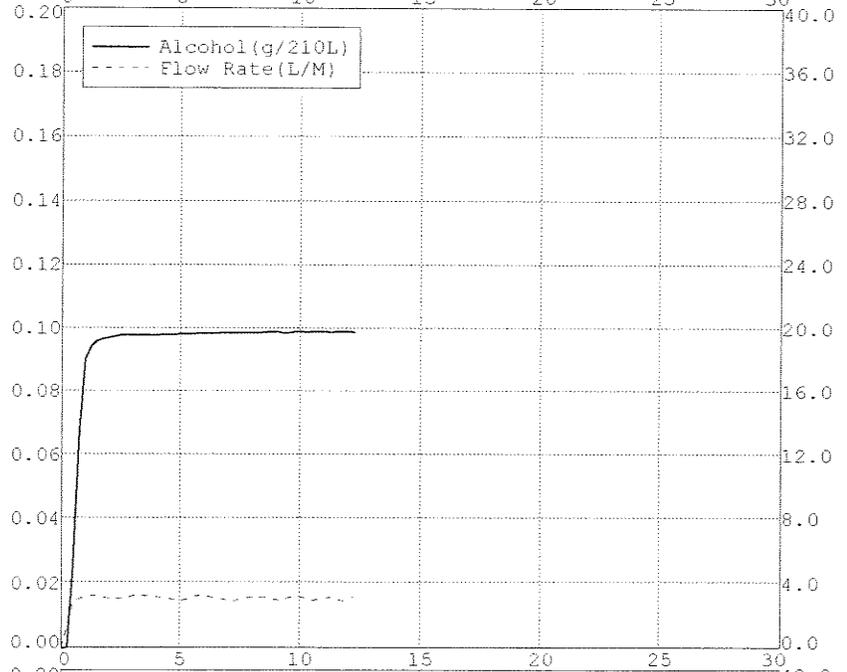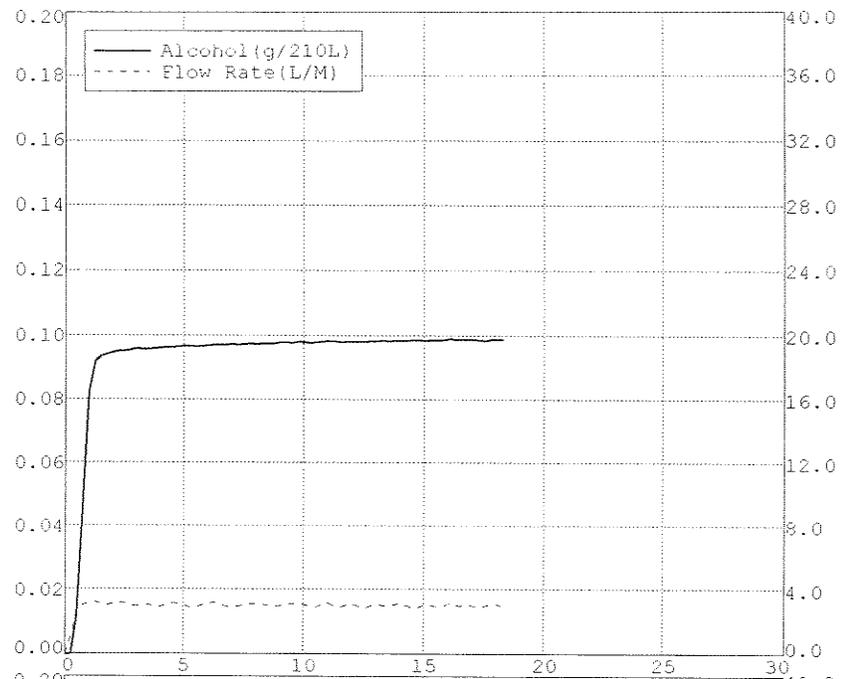

*Sgt. [Signature]* *[Signature]* #24