

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/25/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:04
INTERNAL STANDARD	VERIFIED	14:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:04
BLANK TEST	0.00	14:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:06
BLANK TEST	0.00	14:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:07
BLANK TEST	0.00	14:08

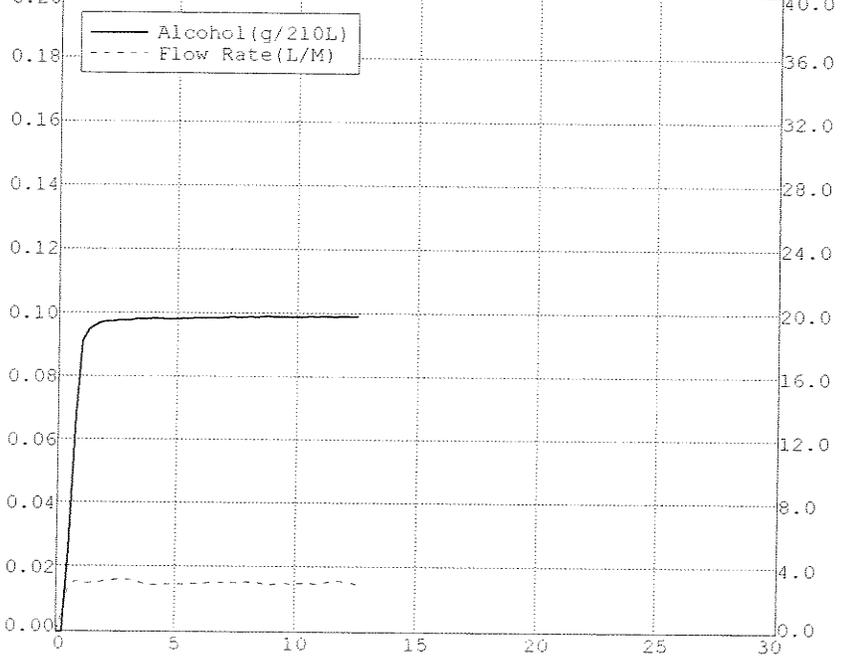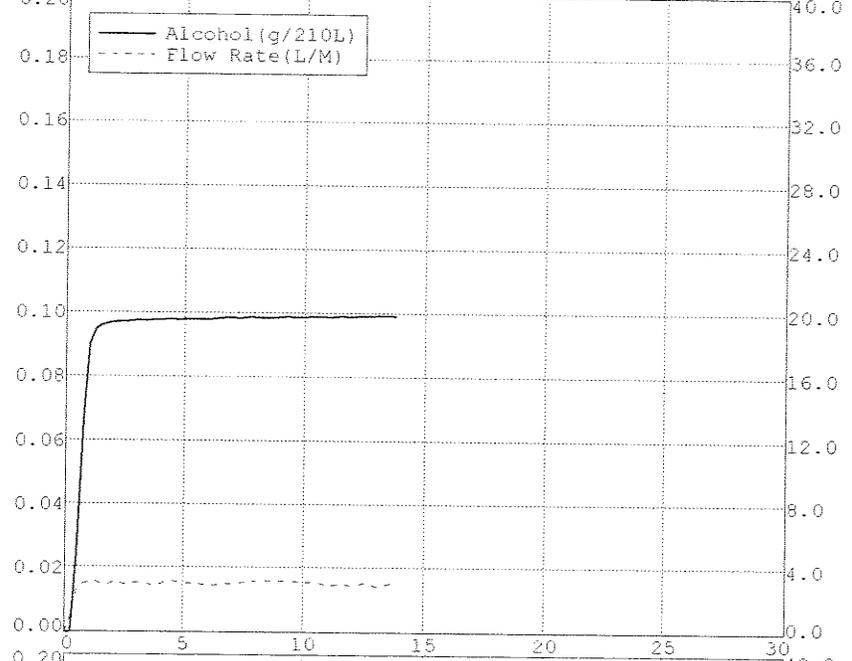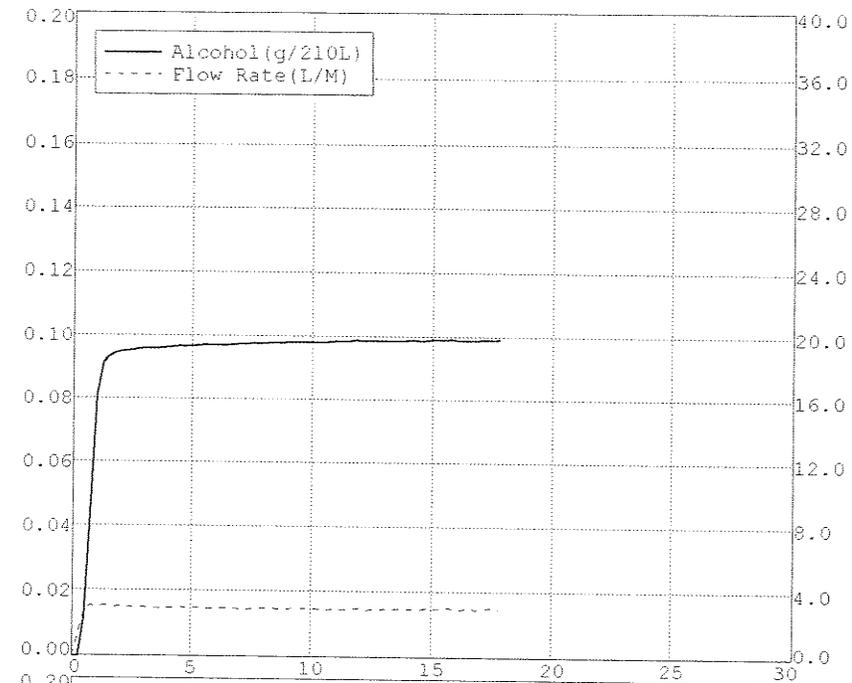

Handwritten signature: J. C. Geisler #241