

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/08/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:55
INTERNAL STANDARD	VERIFIED	08:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:56
BLANK TEST	0.00	08:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:57
BLANK TEST	0.00	08:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	08:58
BLANK TEST	0.00	08:59

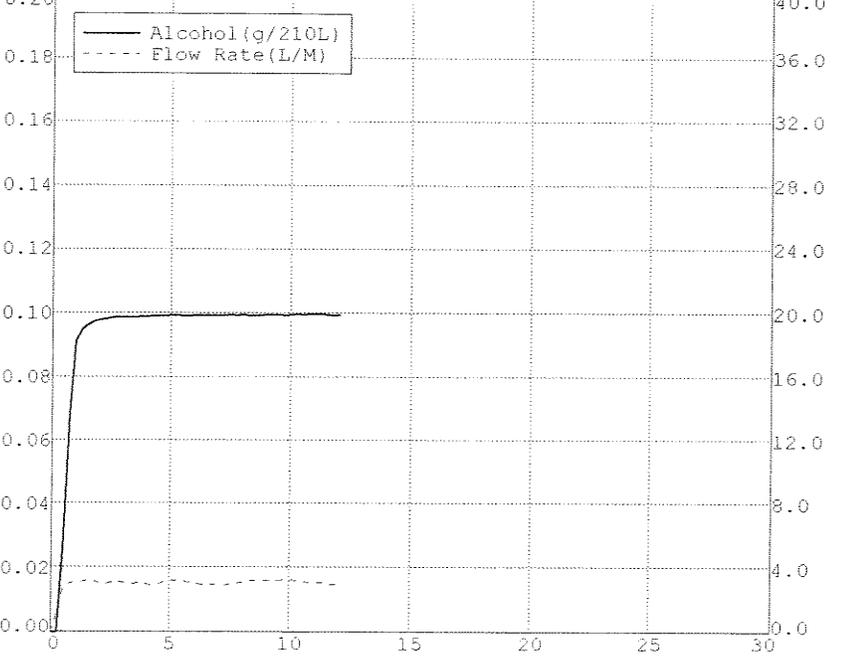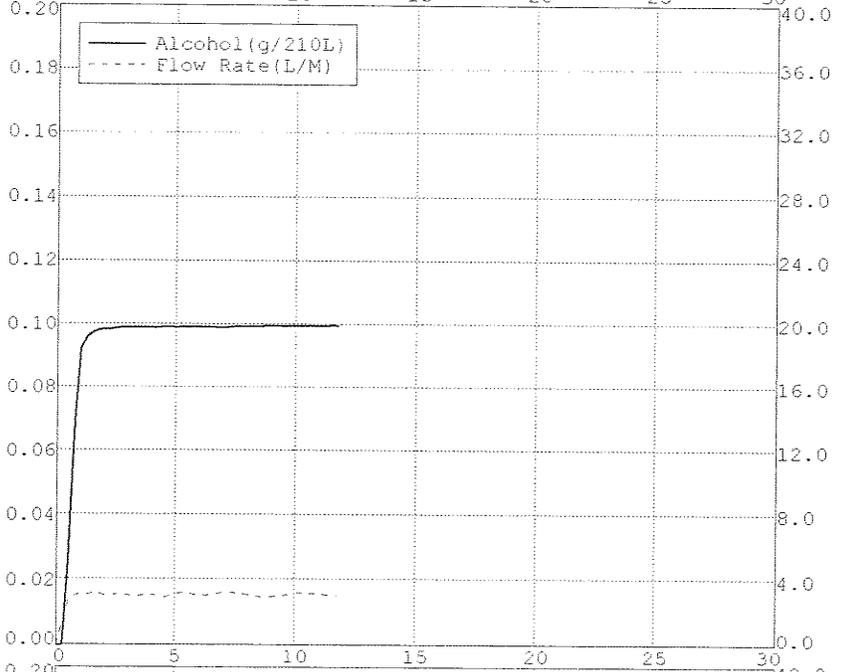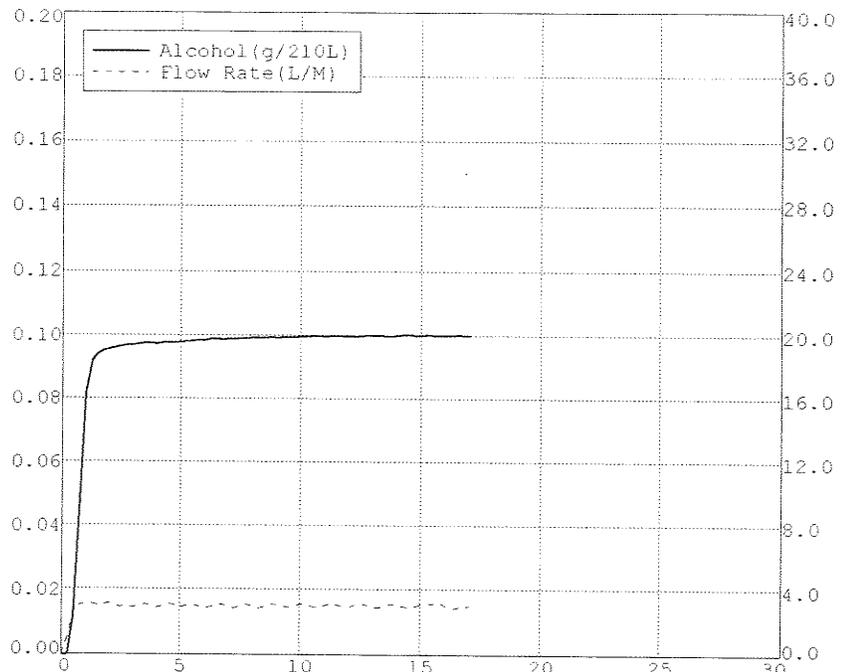

Charles B. Geisler