

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/17/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:34
INTERNAL STANDARD	VERIFIED	14:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:35
BLANK TEST	0.00	14:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:36
BLANK TEST	0.00	14:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:37
BLANK TEST	0.00	14:38

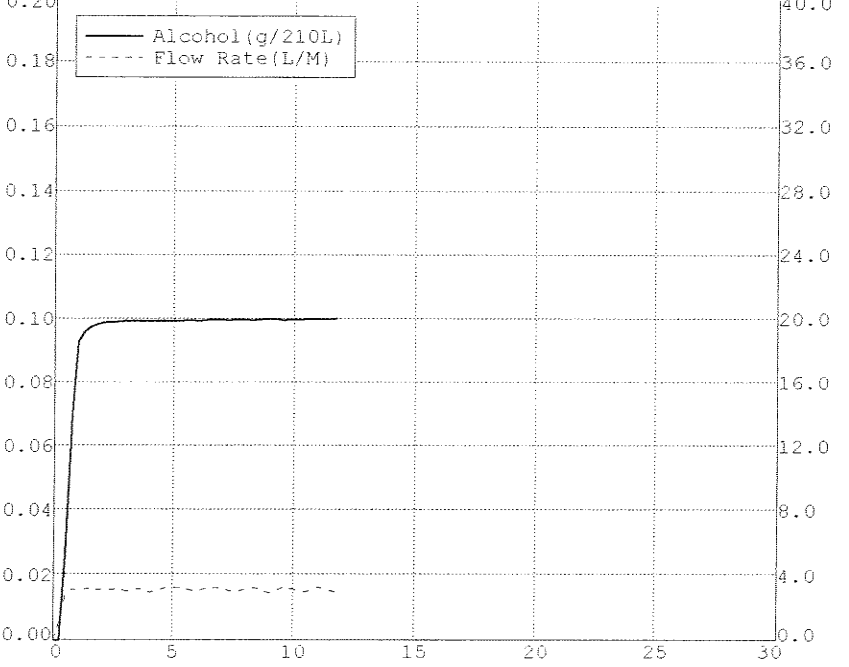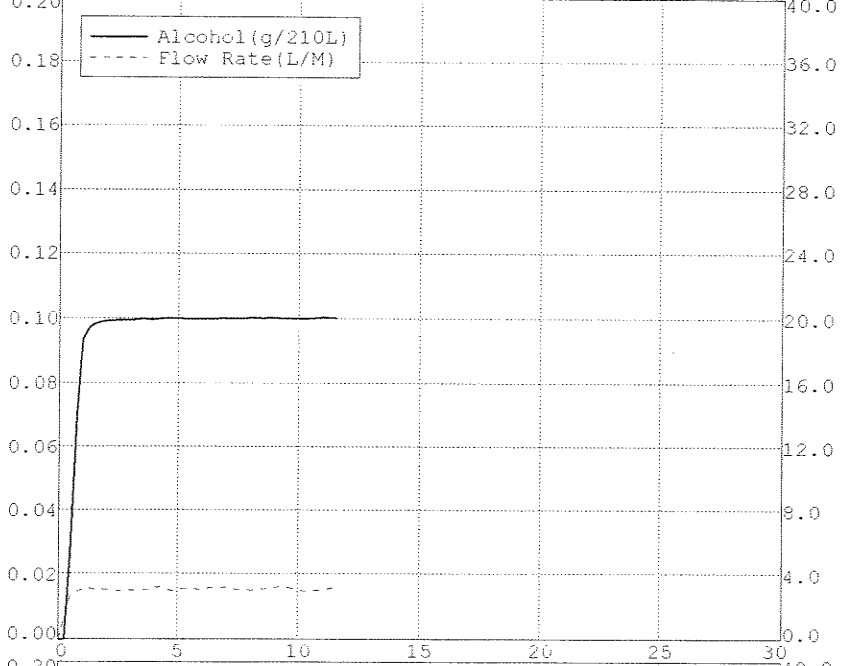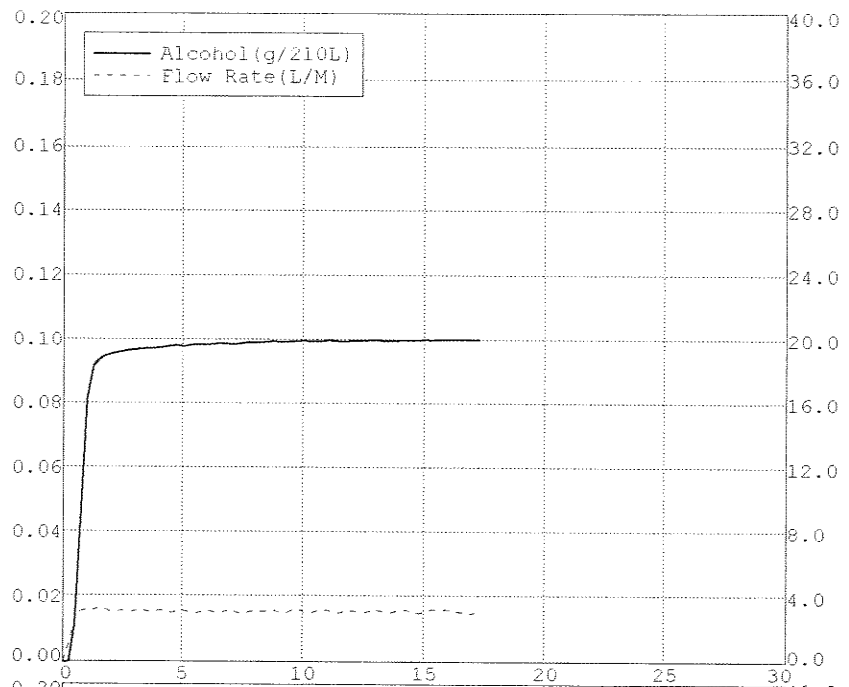

*Charles B. Geisler #241*