

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/23/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:45
INTERNAL STANDARD	VERIFIED	14:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:46
BLANK TEST	0.00	14:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:47
BLANK TEST	0.00	14:48
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:48
BLANK TEST	0.00	14:49

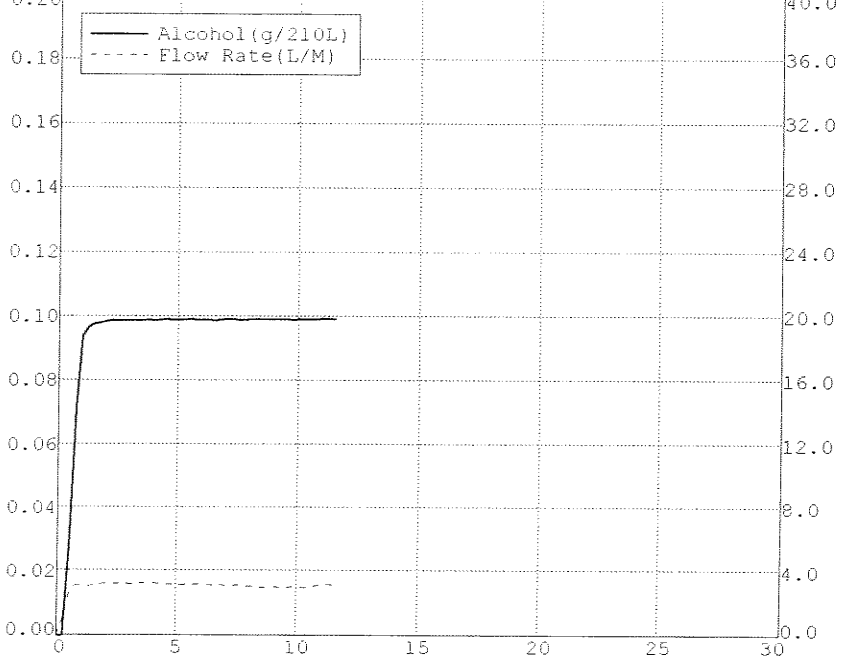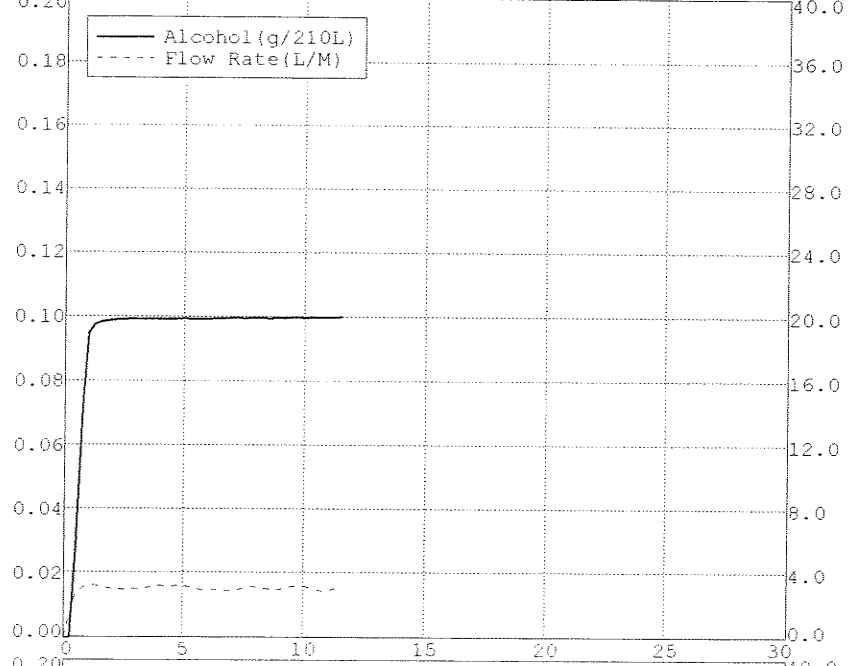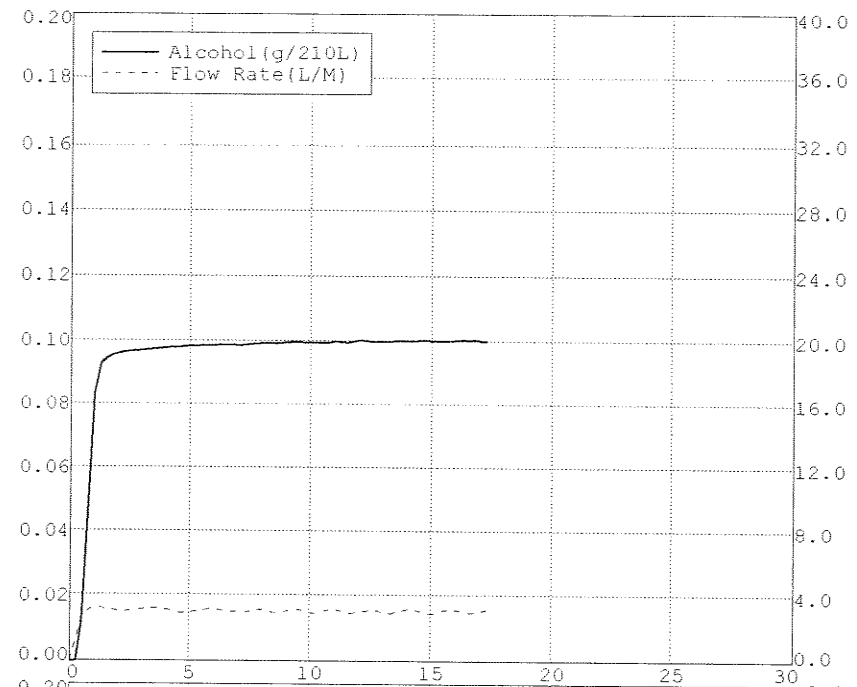

Ch. B. Geisler *[Signature]*