

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/01/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:44
INTERNAL STANDARD	VERIFIED	10:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:45
BLANK TEST	0.00	10:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:46
BLANK TEST	0.00	10:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:47
BLANK TEST	0.00	10:48

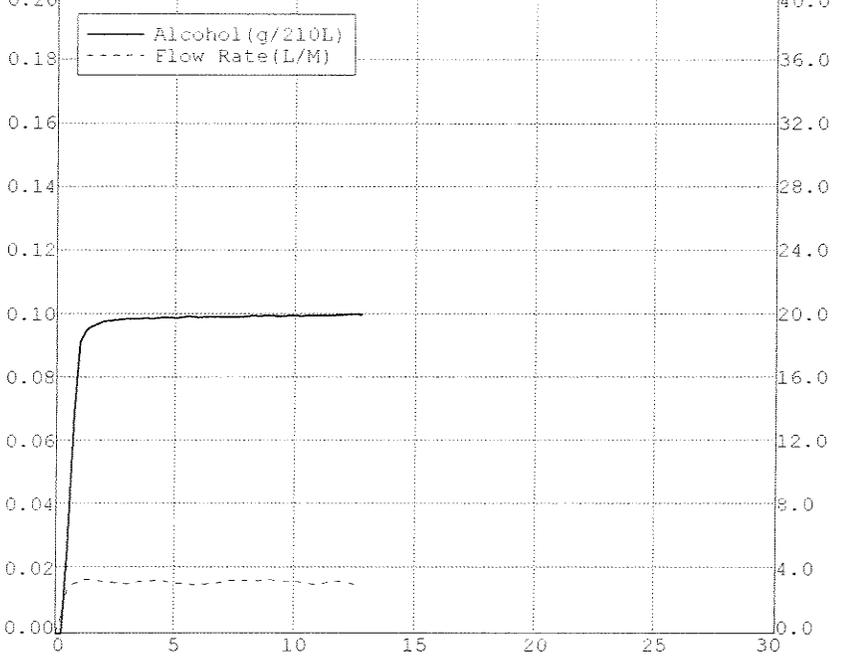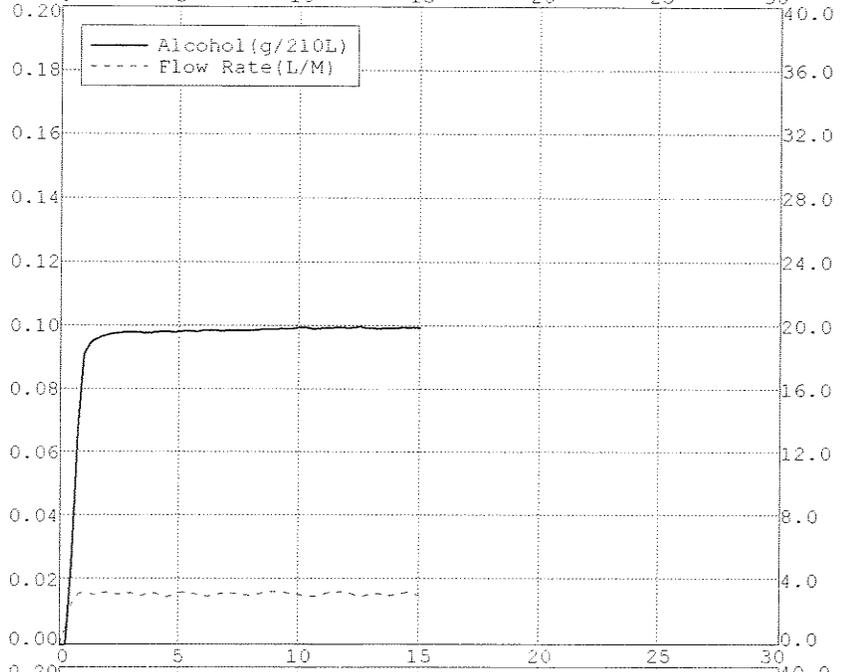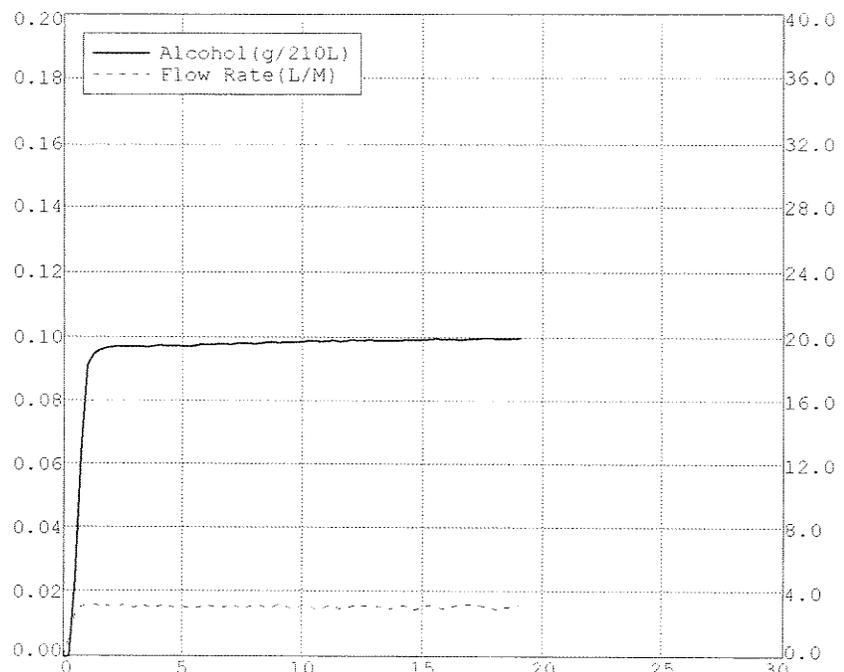

Charles B. Geisler