

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/06/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:05
INTERNAL STANDARD	VERIFIED	09:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:06
BLANK TEST	0.00	09:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:07
BLANK TEST	0.00	09:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:08
BLANK TEST	0.00	09:09

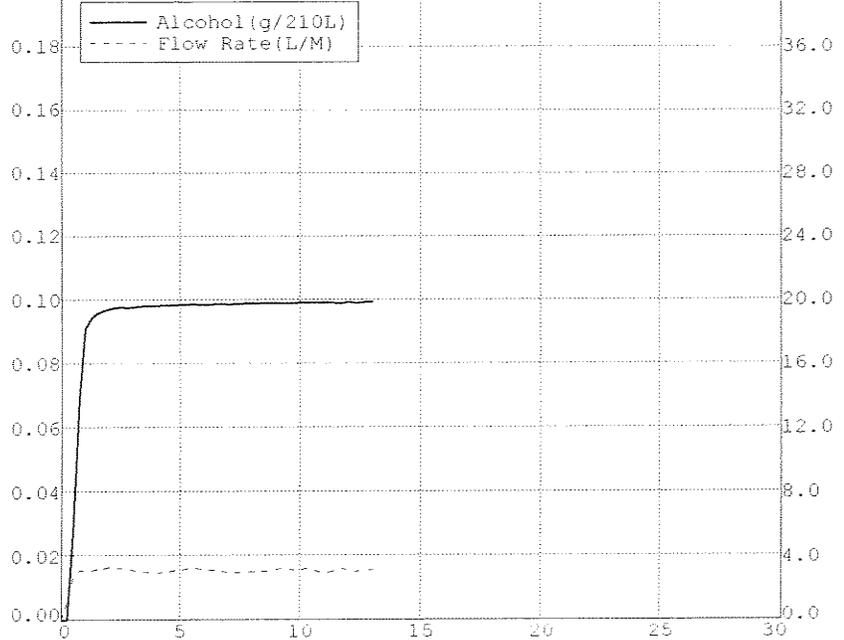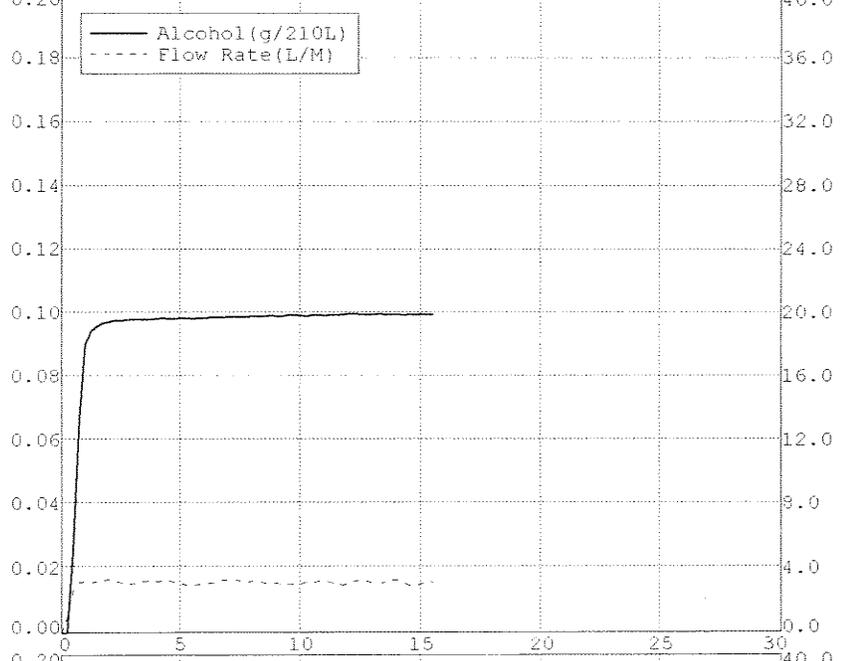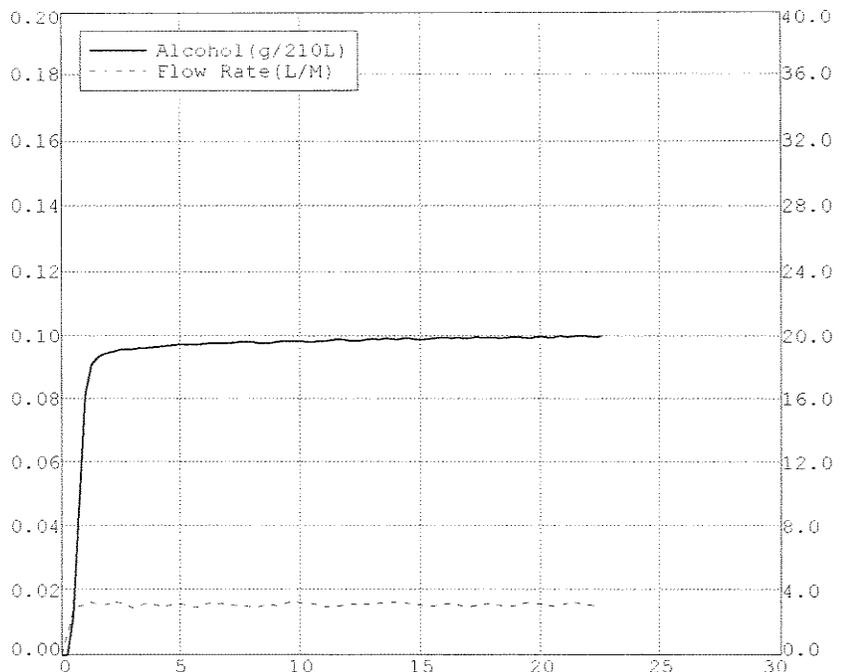

Sgt. Charles B. Geisler #245