

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/14/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:04
INTERNAL STANDARD	VERIFIED	17:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:04
BLANK TEST	0.00	17:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	17:06
BLANK TEST	0.00	17:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	17:07
BLANK TEST	0.00	17:08

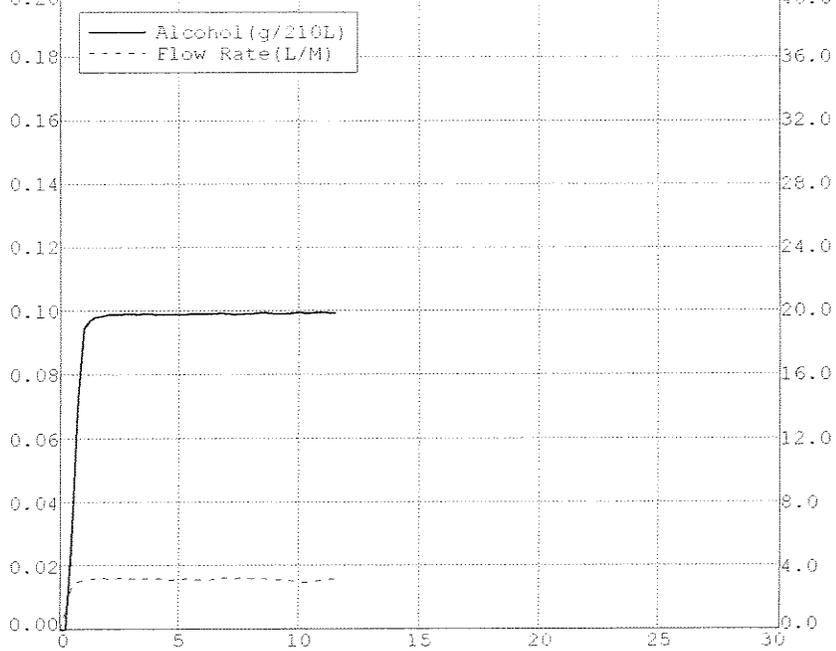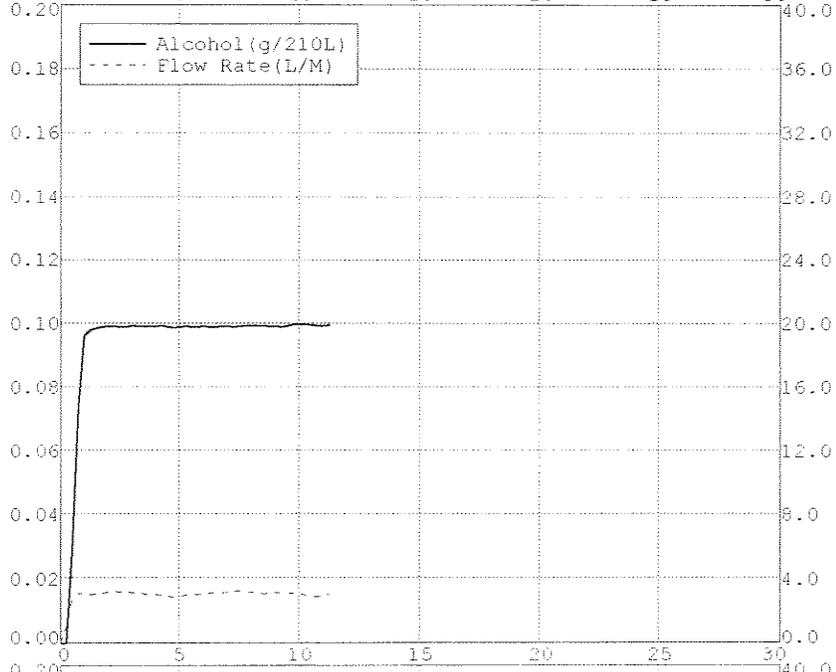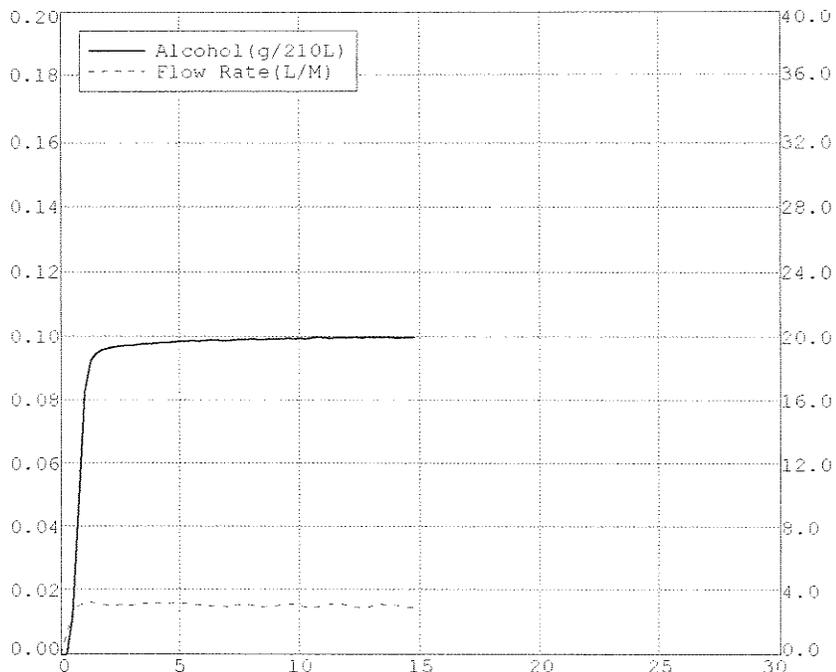

Handwritten signature: C. B. Geisler