

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/20/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:11
INTERNAL STANDARD	VERIFIED	09:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:11
BLANK TEST	0.00	09:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	09:13
BLANK TEST	0.00	09:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	09:14
BLANK TEST	0.00	09:15

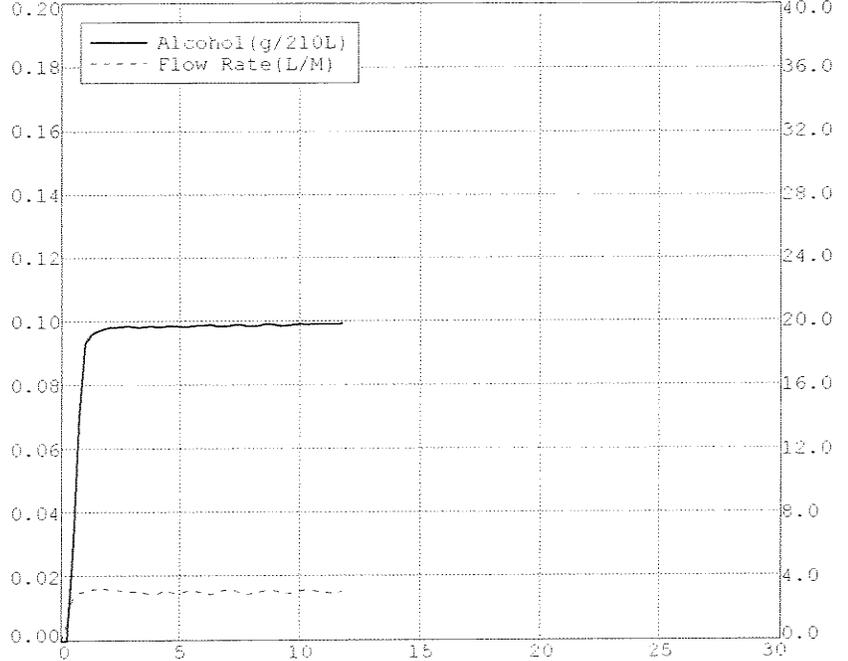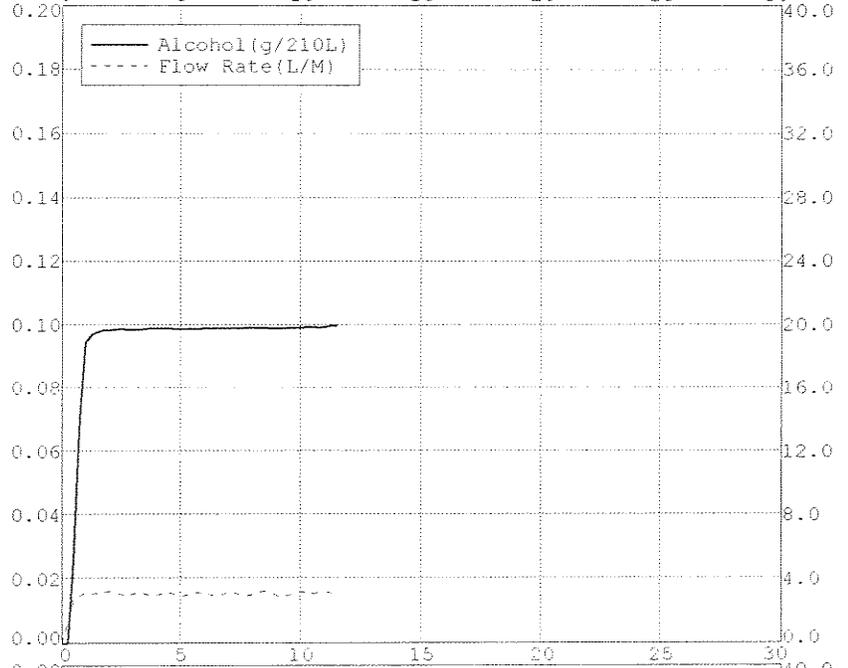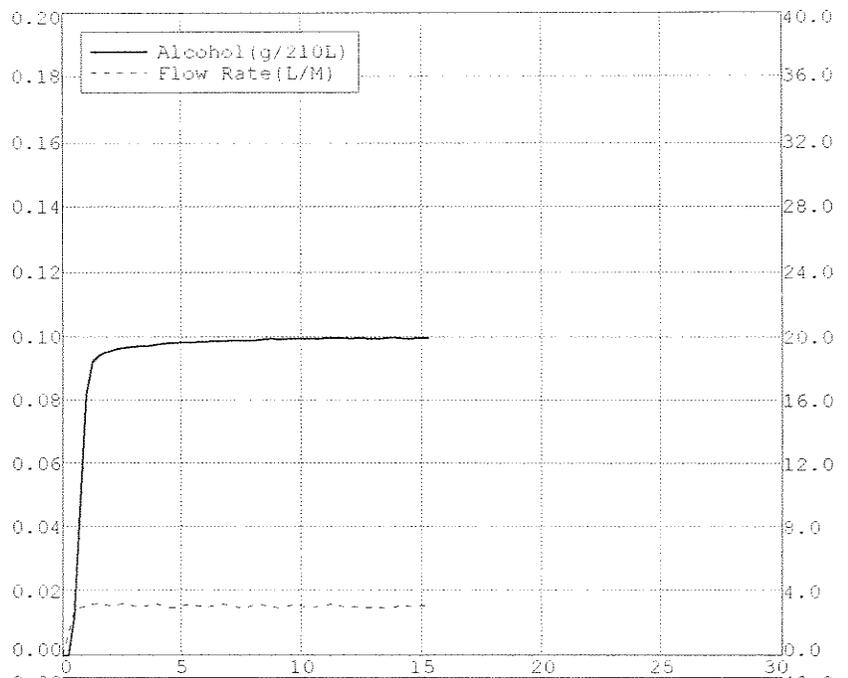

Sgt. C. B. Geisler #2416