

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/02/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:42
INTERNAL STANDARD	VERIFIED	13:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:42
BLANK TEST	0.00	13:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:43
BLANK TEST	0.00	13:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:44
BLANK TEST	0.00	13:45

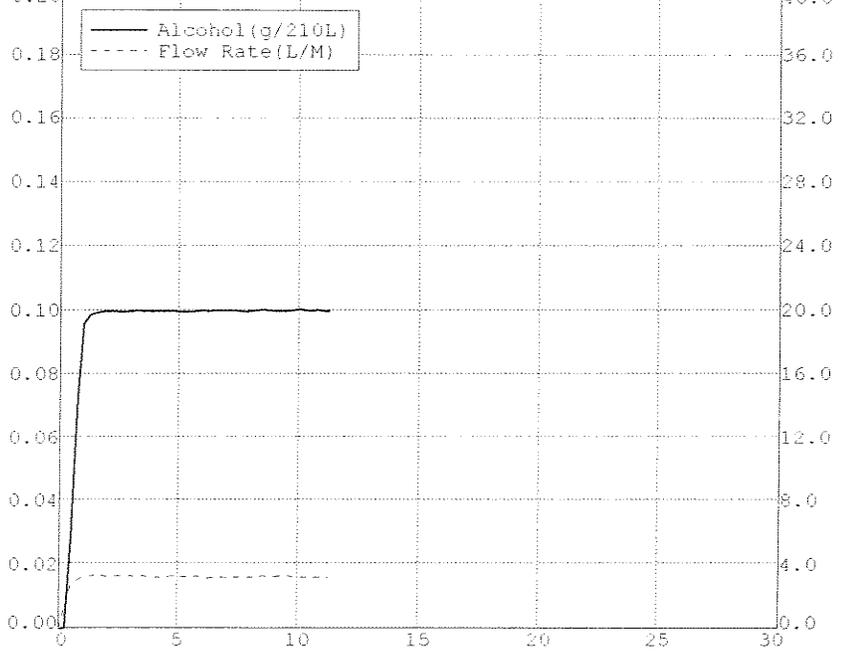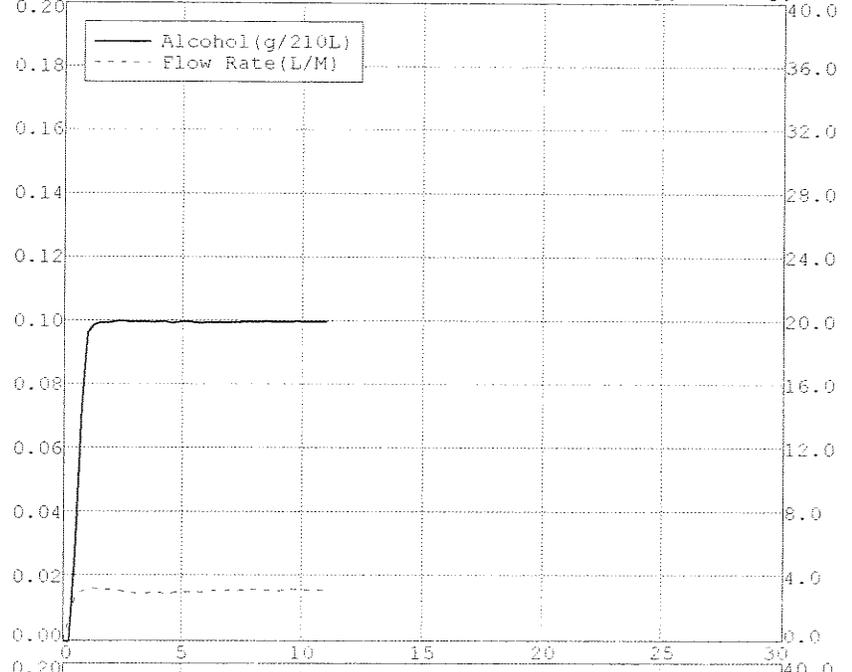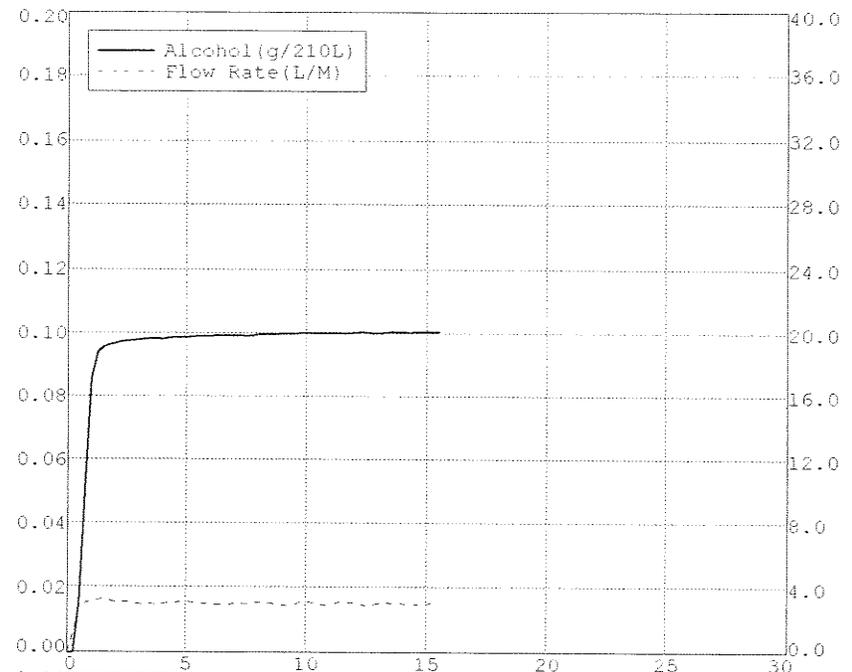

*Charles B Geisler*