

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 07/09/2021

OPERATOR NAME:
 MICHAEL A CAMPBELL
 Permit #: 42422
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:16
INTERNAL STANDARD	VERIFIED	03:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	03:16
BLANK TEST	0.00	03:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:18
BLANK TEST	0.00	03:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:19
BLANK TEST	0.00	03:20

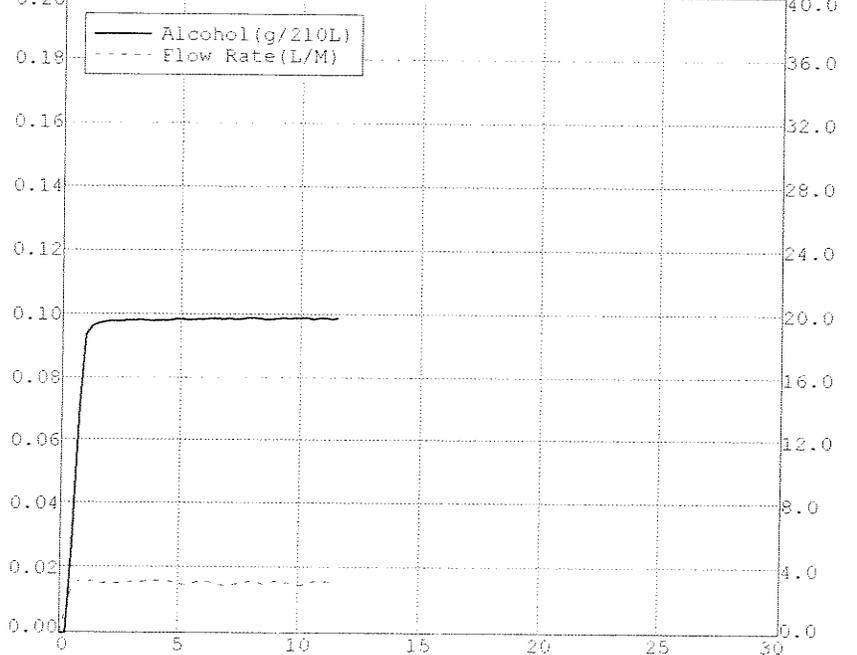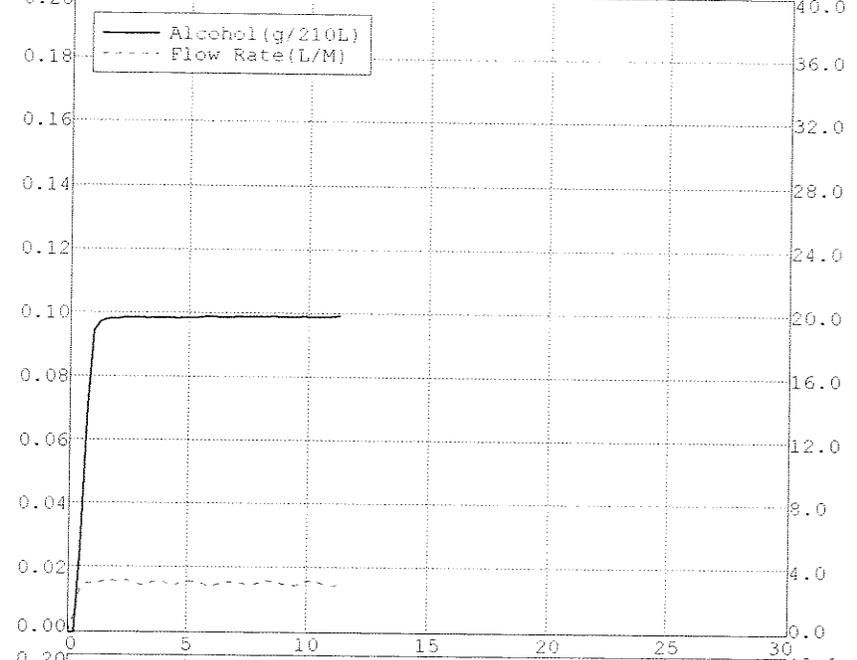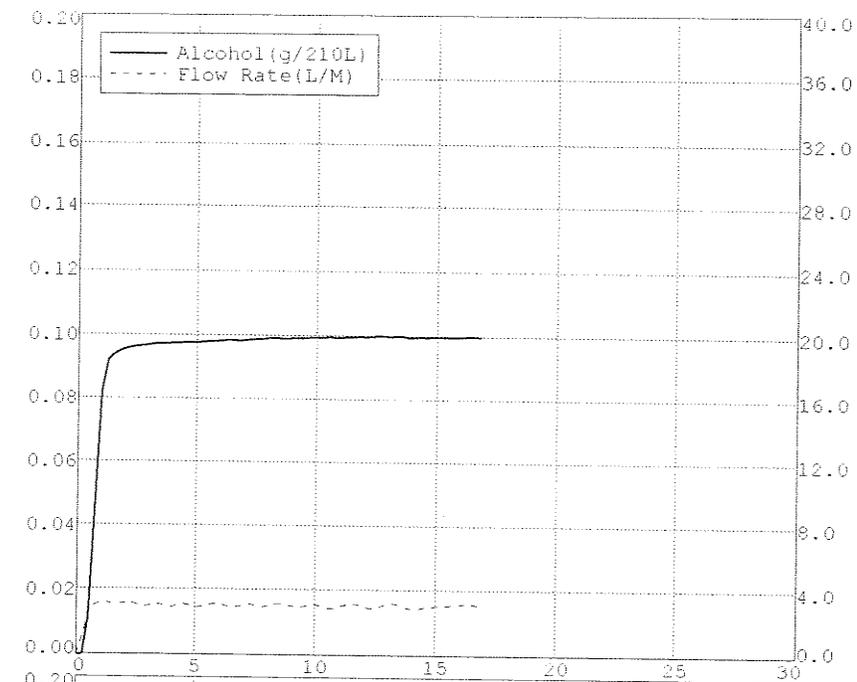

PO Michael Campbell #757