

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/09/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21170

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 15:24 |
| INTERNAL STANDARD | VERIFIED | 15:24 |
| REFERENCE STANDARD TEMP | 34.01c | |
| REFERENCE STANDARD | 0.10 | 15:24 |
| BLANK TEST | 0.00 | 15:25 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 15:25 |
| BLANK TEST | 0.00 | 15:26 |
| REFERENCE STANDARD TEMP | 34.02c | |
| REFERENCE STANDARD | 0.10 | 15:26 |
| BLANK TEST | 0.00 | 15:27 |

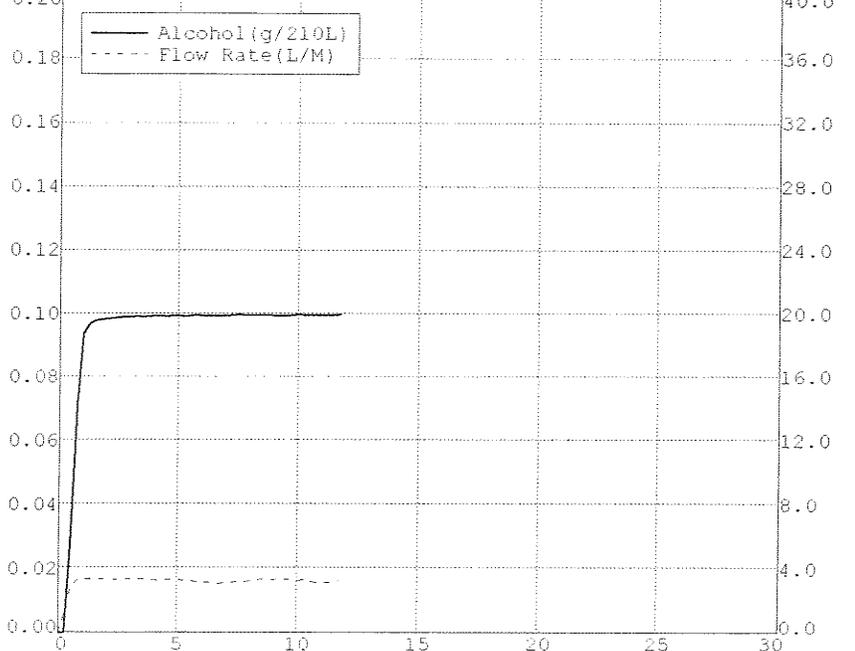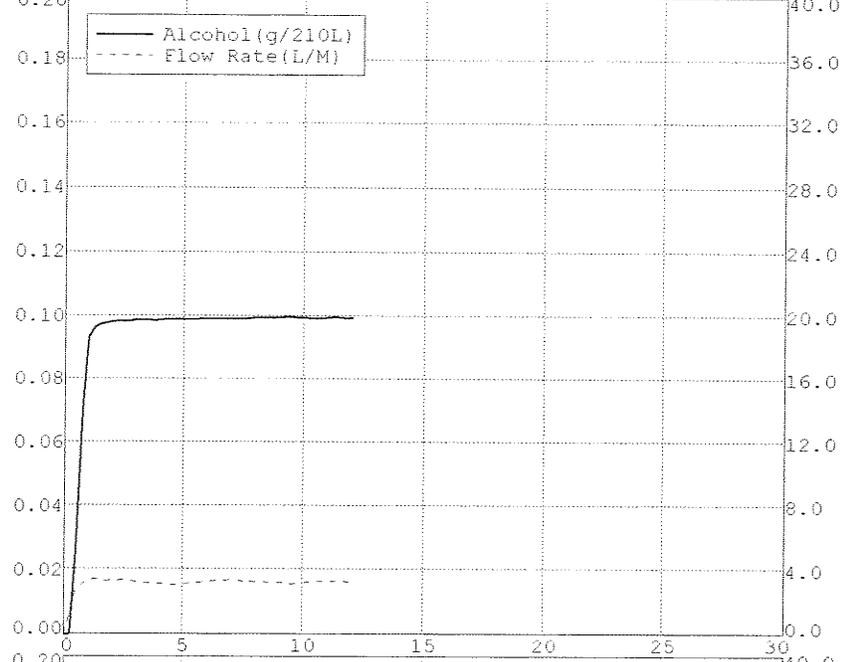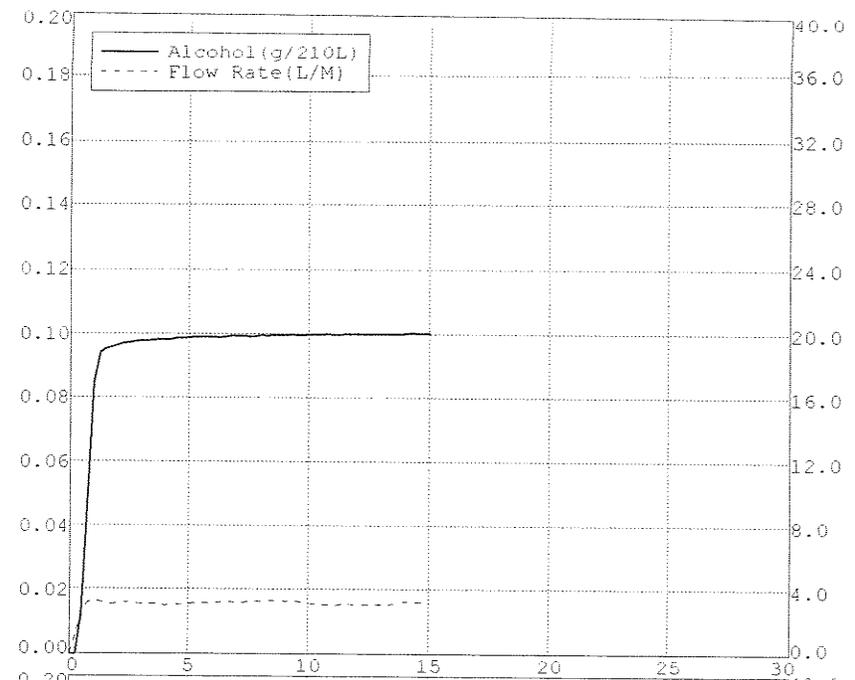

Sp. Ch. B. Geisler #211