

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 08/23/2021

OPERATOR NAME:  
SEAN T SMITH  
Permit #: 46227  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	07:51
INTERNAL STANDARD	VERIFIED	07:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	07:52
BLANK TEST	0.00	07:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	07:53
BLANK TEST	0.00	07:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	07:54
BLANK TEST	0.00	07:55

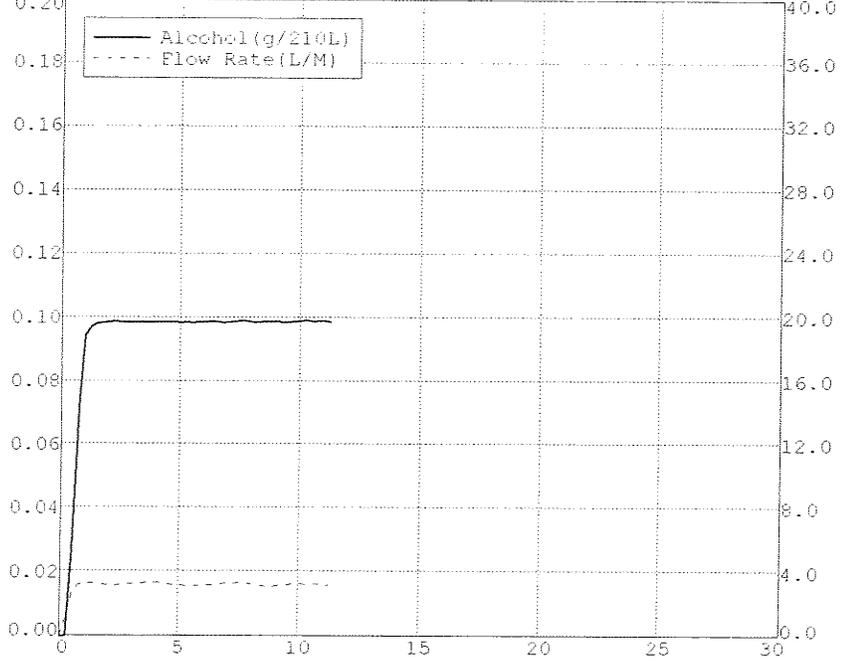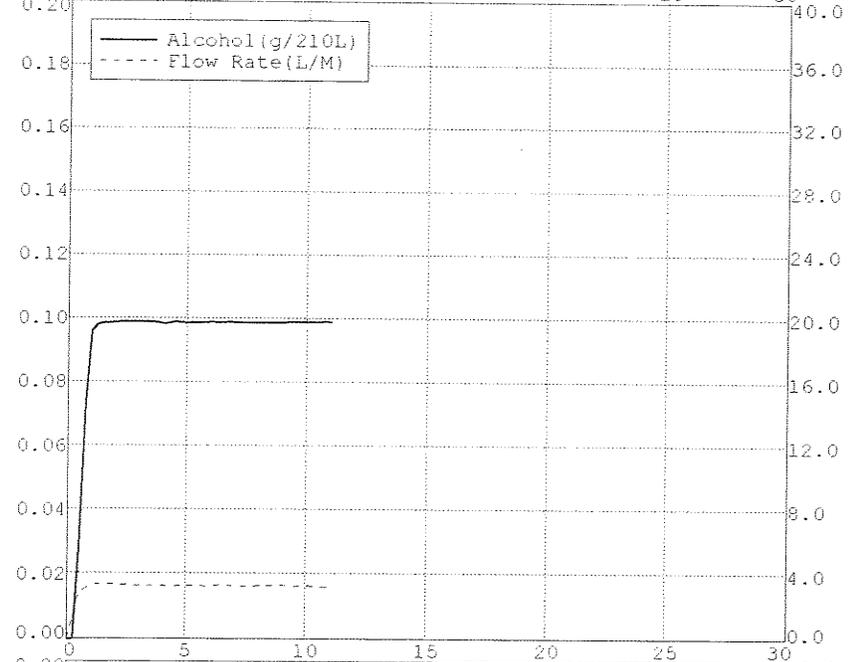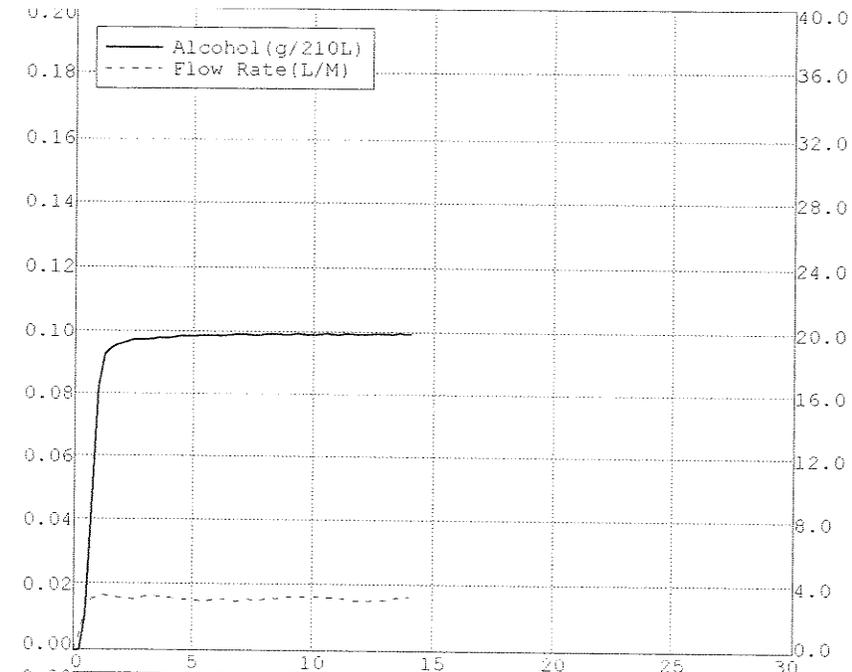

*Handwritten signature and initials*