

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/29/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:05
INTERNAL STANDARD	VERIFIED	16:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	16:05
BLANK TEST	0.00	16:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:07
BLANK TEST	0.00	16:08
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	16:08
BLANK TEST	0.00	16:09

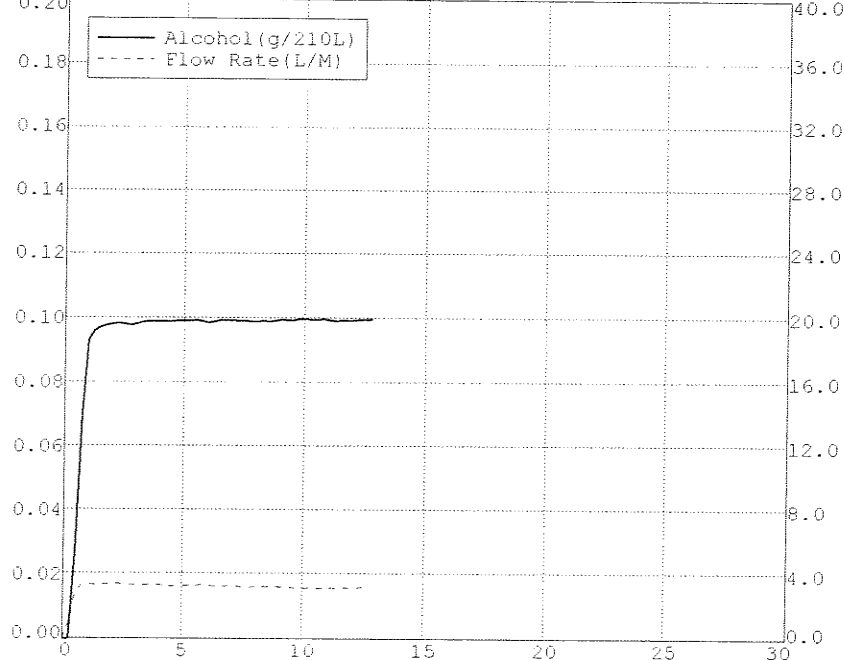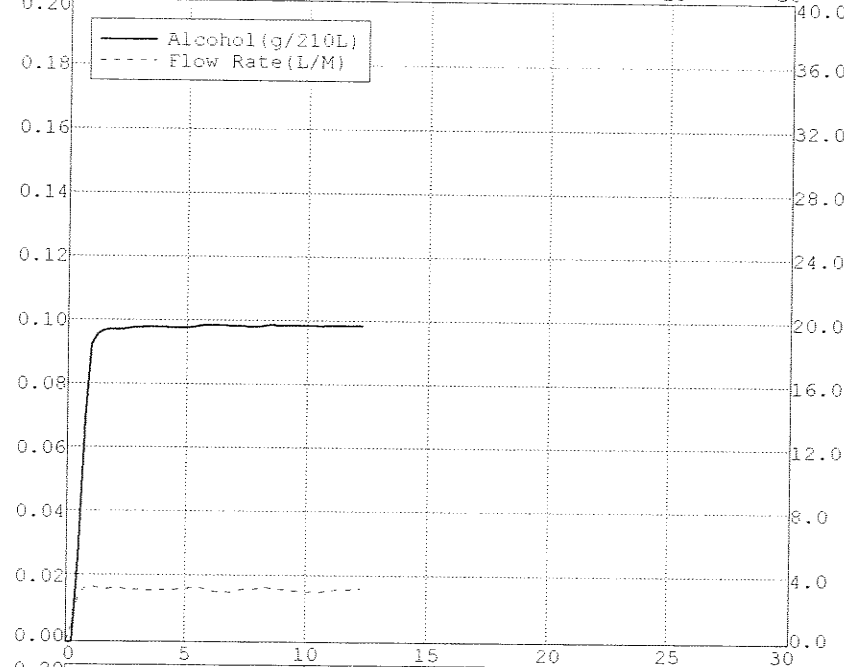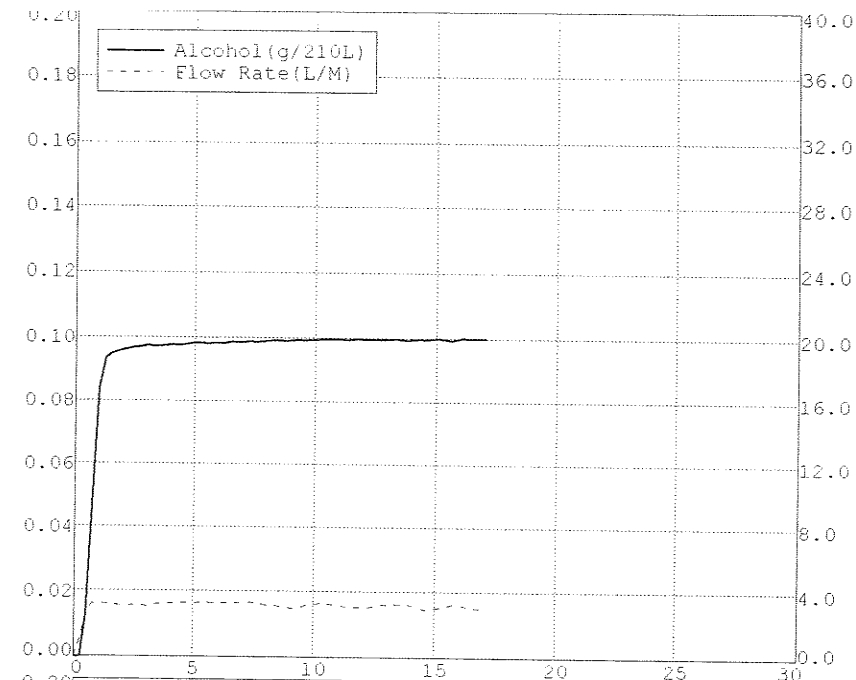

Signature: Sgt. Charles B. Geisler