

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/25/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21170

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:13
INTERNAL STANDARD	VERIFIED	18:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	18:13
BLANK TEST	0.00	18:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:15
BLANK TEST	0.00	18:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:17

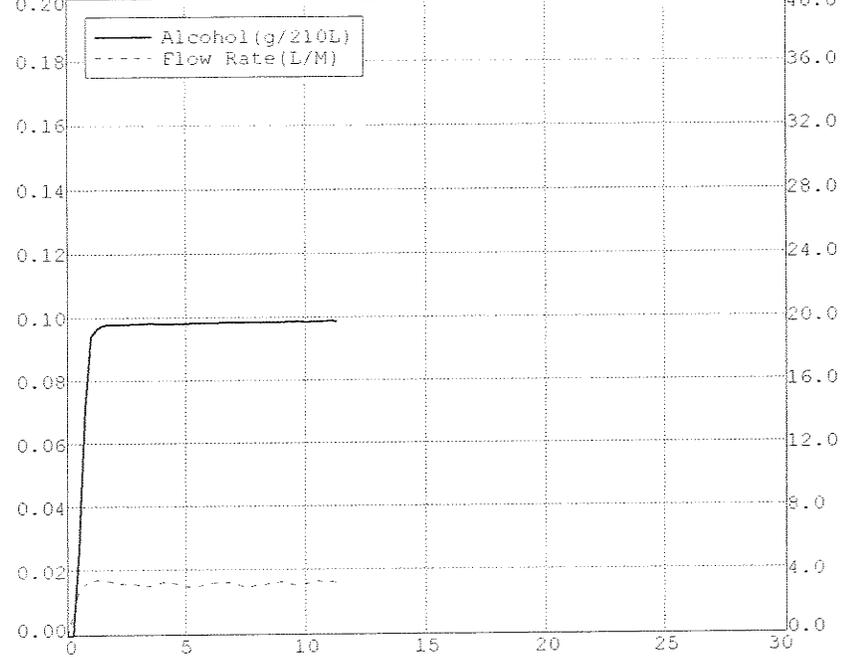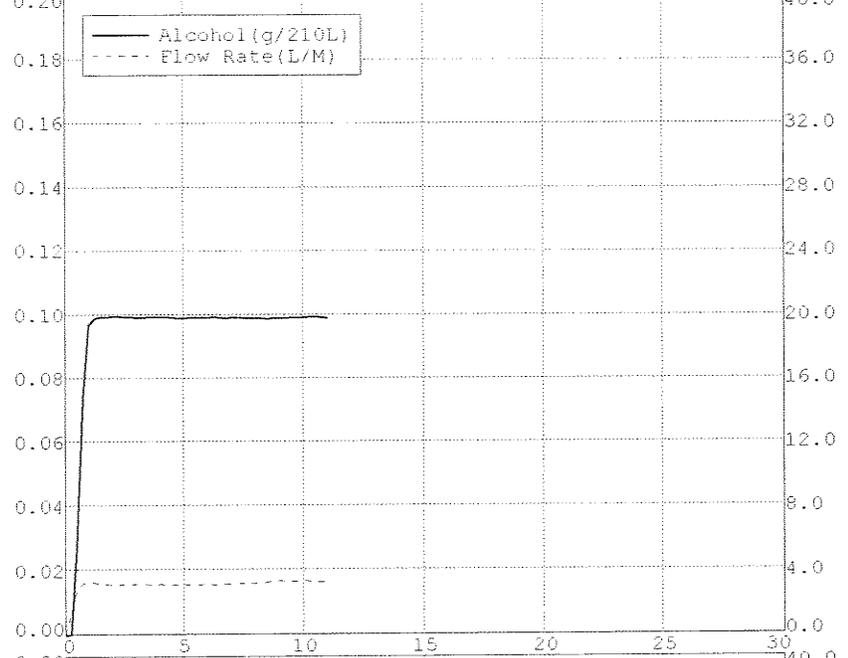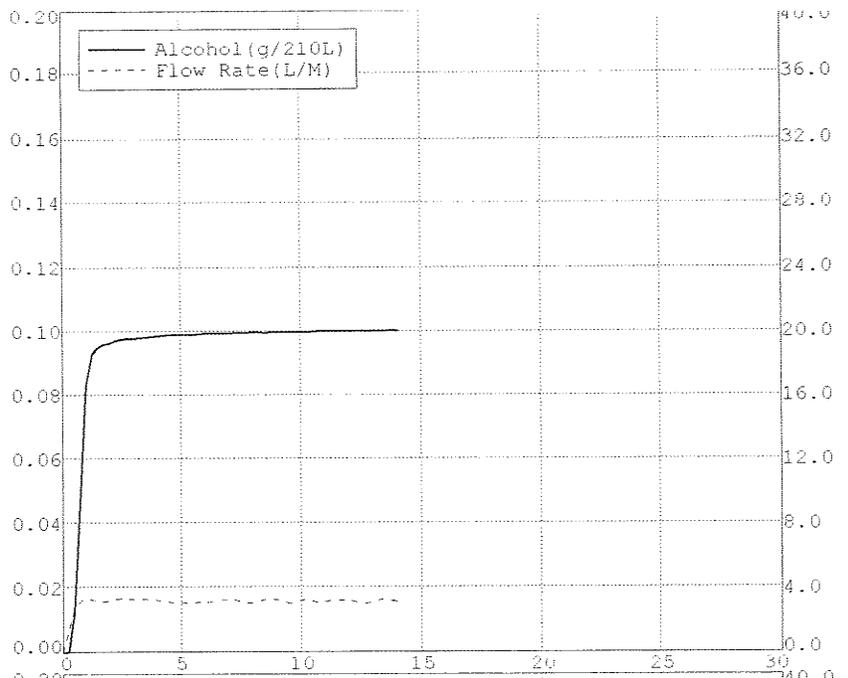

Sgt. C.B. Geisler #201