

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 10/01/2021

OPERATOR NAME:  
J RIEHL  
Permit #: 47503  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:03
INTERNAL STANDARD	VERIFIED	04:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:03
BLANK TEST	0.00	04:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:05
BLANK TEST	0.00	04:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:06
BLANK TEST	0.00	04:07

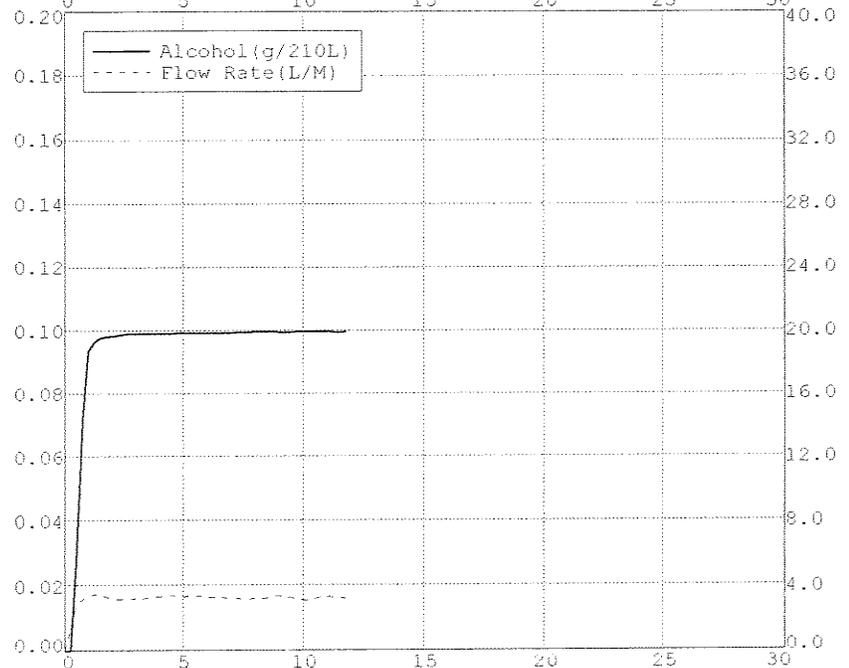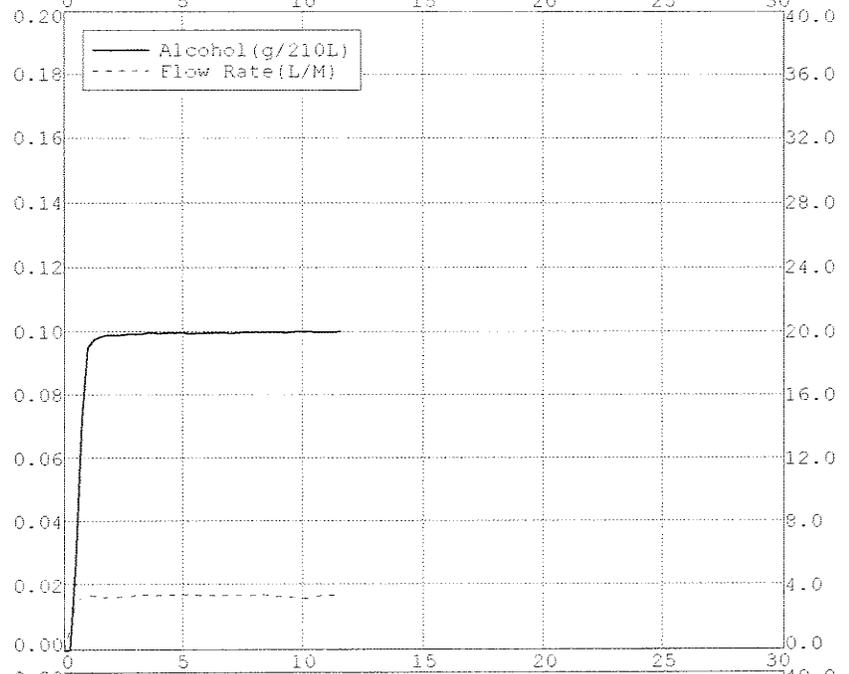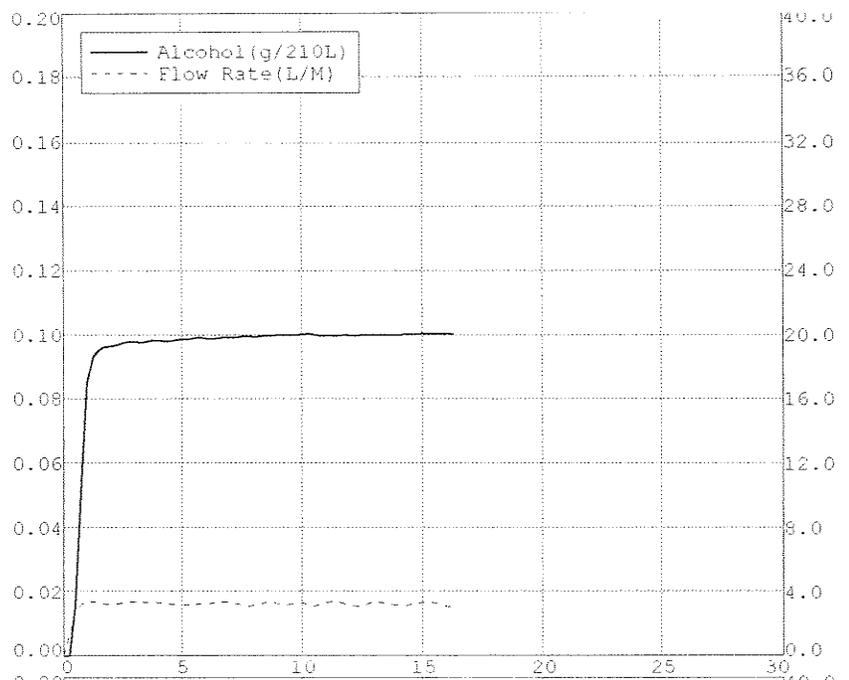

*J Riehl*  
#820