

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/09/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:56
INTERNAL STANDARD	VERIFIED	10:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:56
BLANK TEST	0.00	10:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:57
BLANK TEST	0.00	10:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:59
BLANK TEST	0.00	11:00

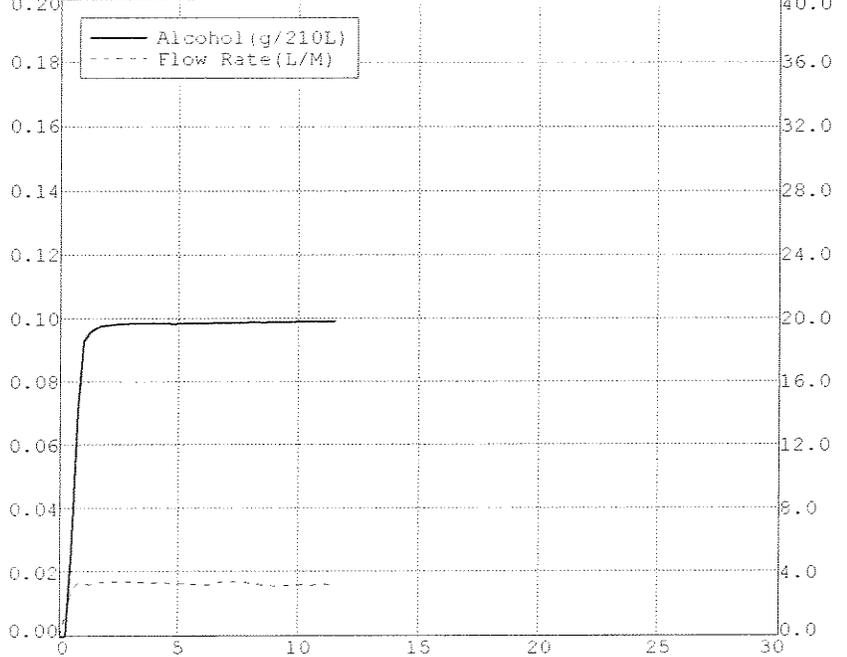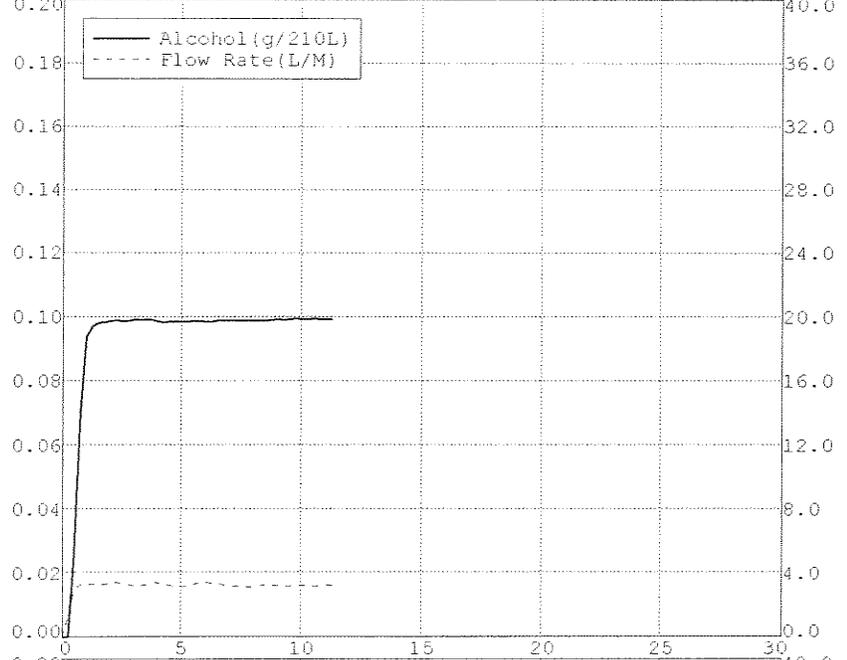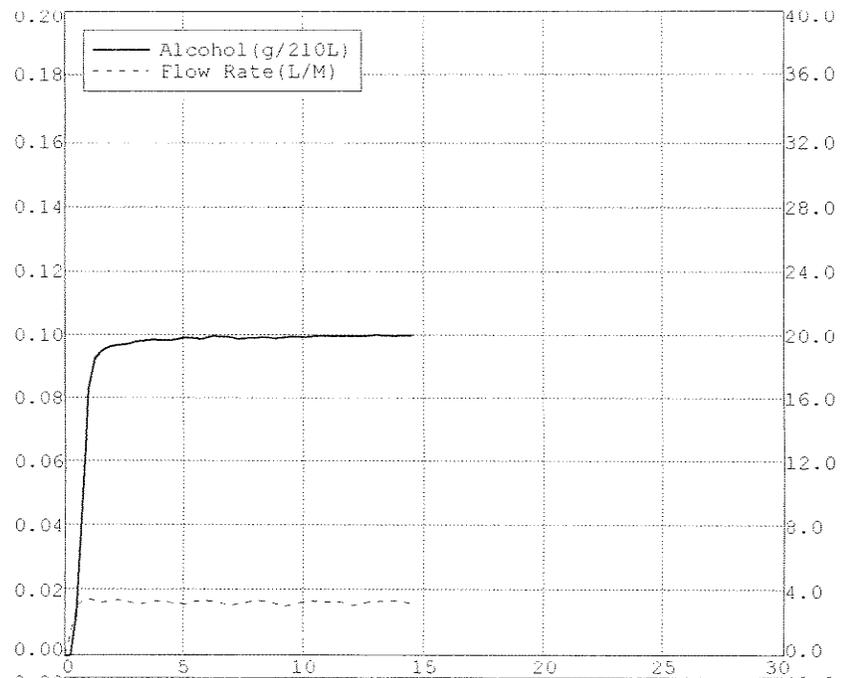

Charles B Geisler
#201