

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/24/2021

OPERATOR NAME:
SEAN T SMITH
Permit #: 46227
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:19
INTERNAL STANDARD	VERIFIED	08:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:19
BLANK TEST	0.00	08:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:21
BLANK TEST	0.00	08:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:22
BLANK TEST	0.00	08:23

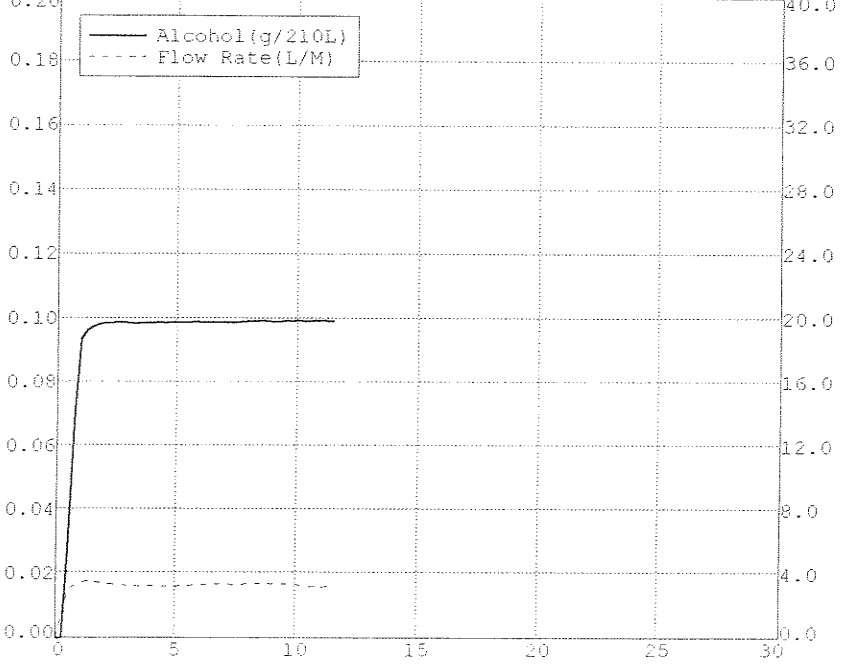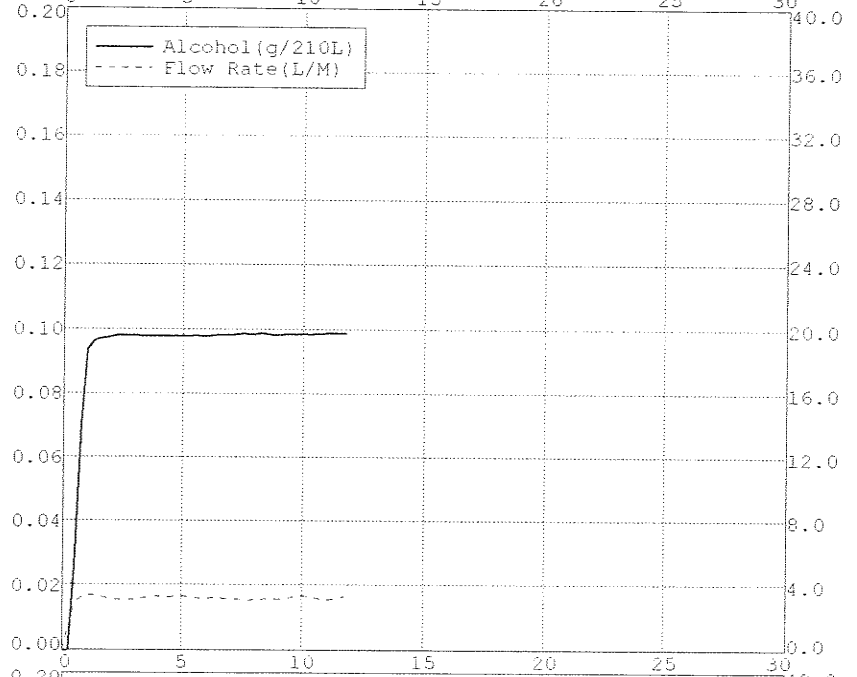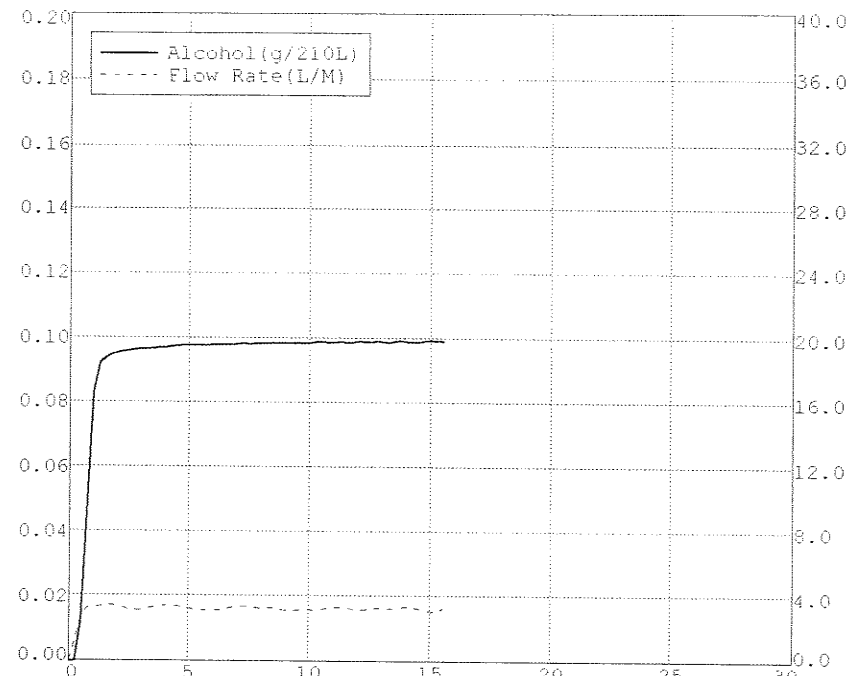

Handwritten signature