

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 11/07/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:57
INTERNAL STANDARD	VERIFIED	10:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	10:57
BLANK TEST	0.00	10:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	10:59
BLANK TEST	0.00	10:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	11:00
BLANK TEST	0.00	11:01

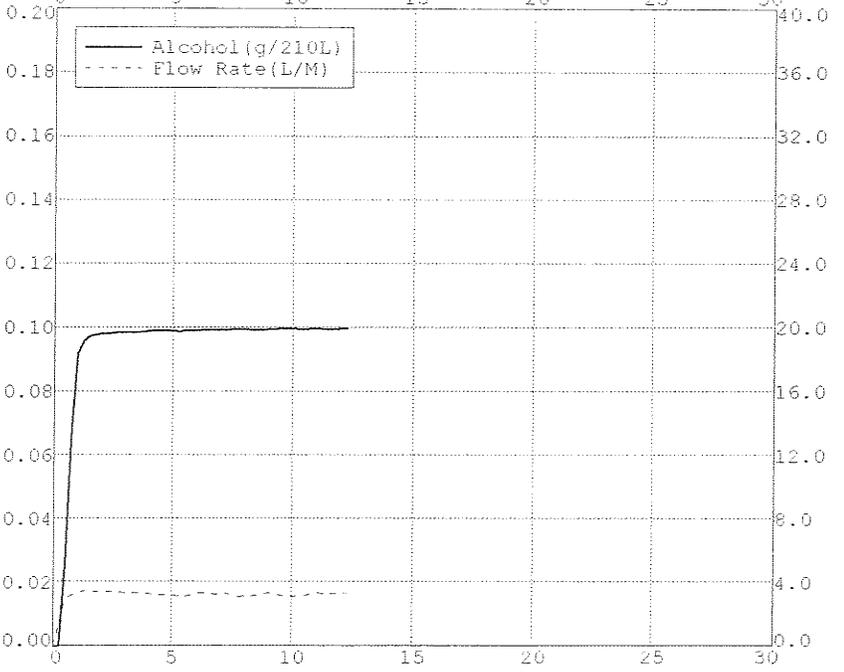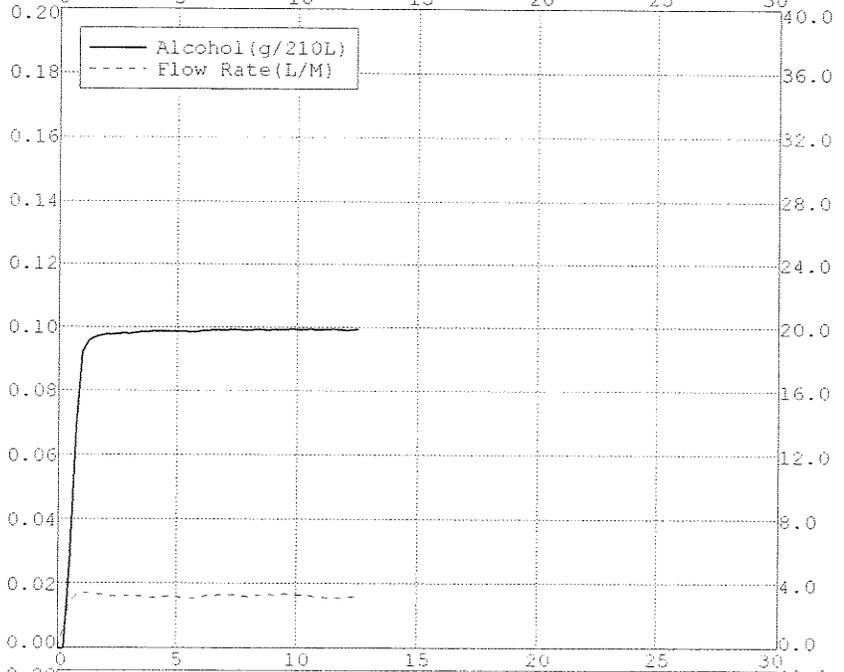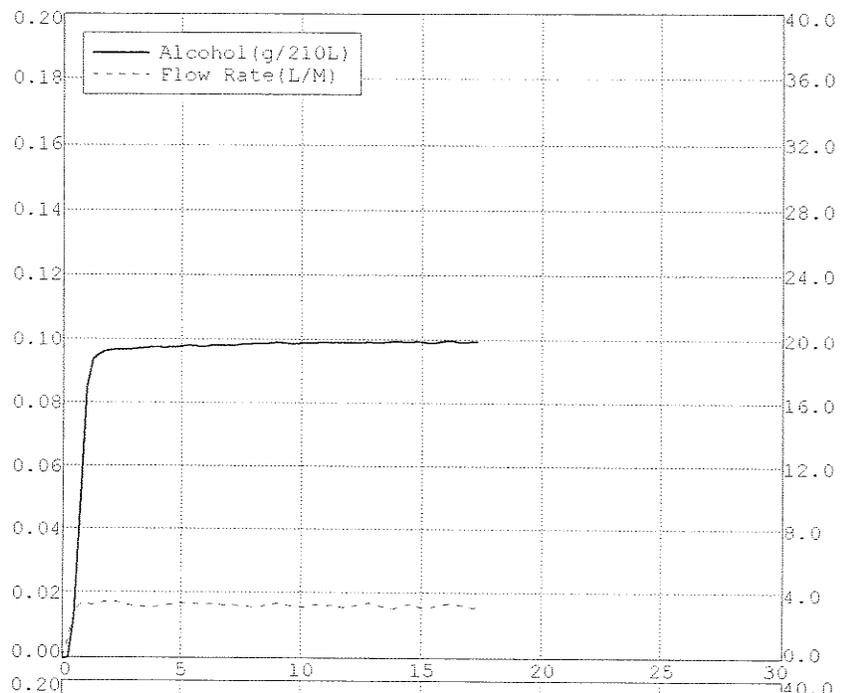

Charles B. Geisler #241