

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 11/24/2021

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 21280

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:18
INTERNAL STANDARD	VERIFIED	13:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:18
BLANK TEST	0.00	13:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:19
BLANK TEST	0.00	13:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:21
BLANK TEST	0.00	13:22

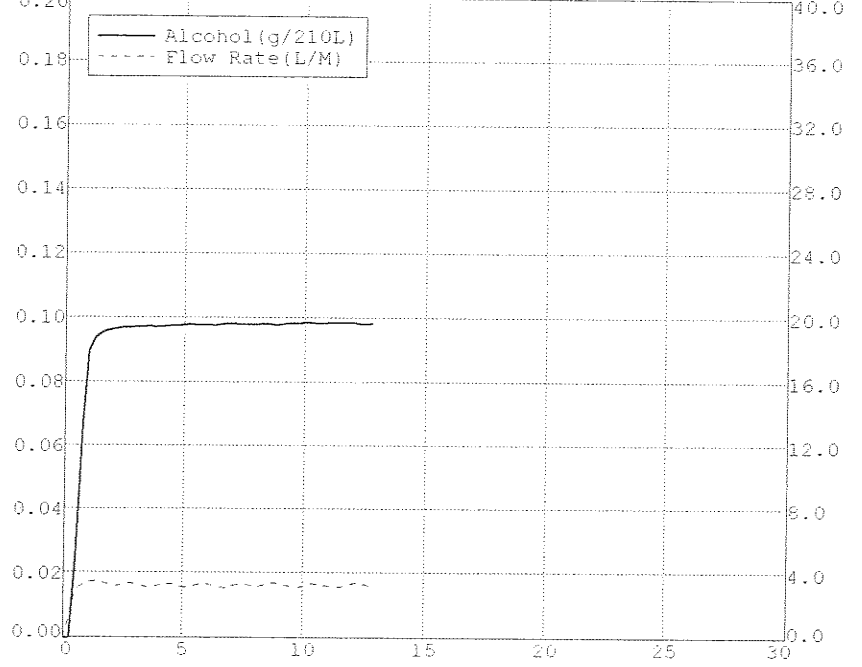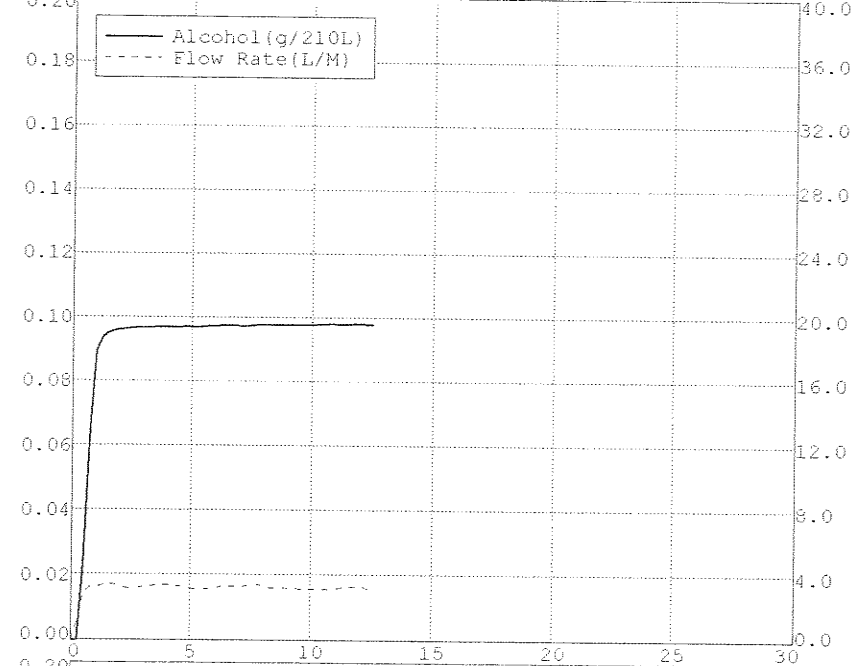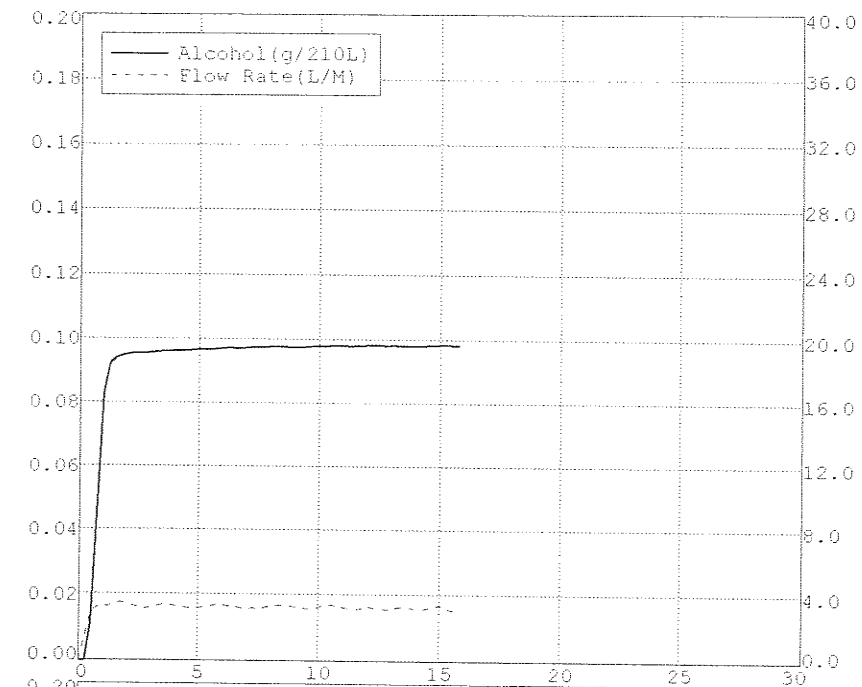

*Handwritten signatures and initials:*  
 C.B. Geisler, [Signature], #24