

SOLUTION CHANGE




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 01/01/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:51
INTERNAL STANDARD	VERIFIED	15:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:51
BLANK TEST	0.00	15:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:53
BLANK TEST	0.00	15:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:54
BLANK TEST	0.00	15:55

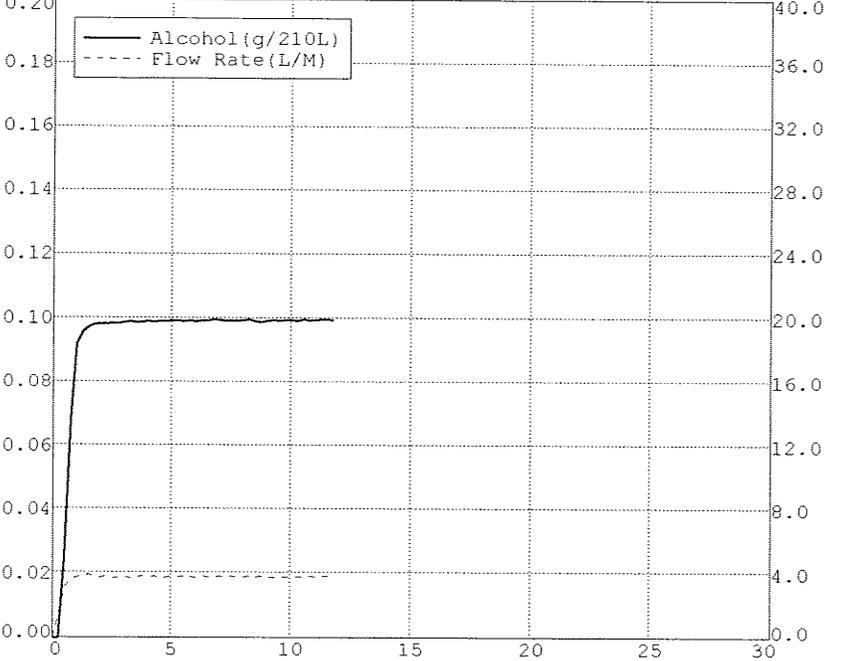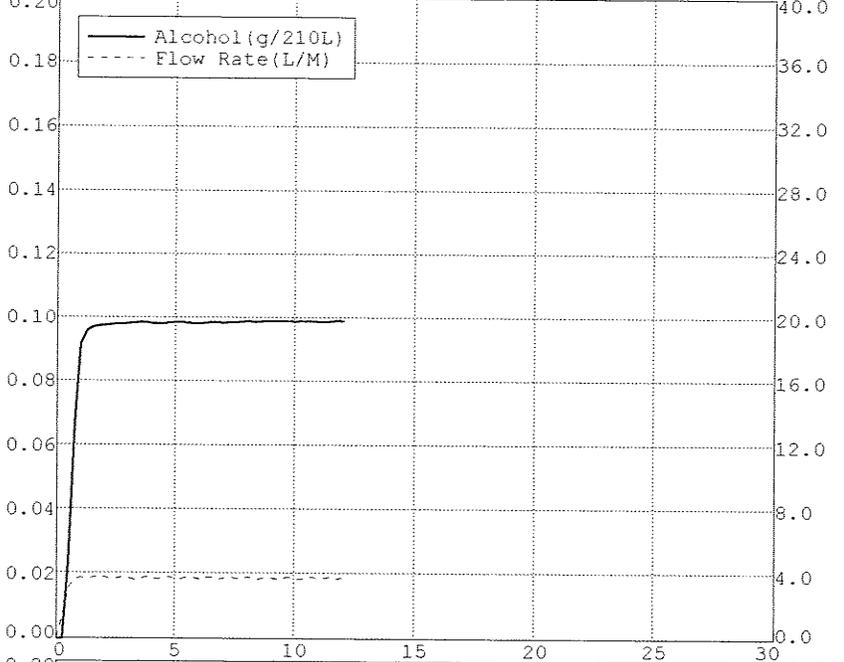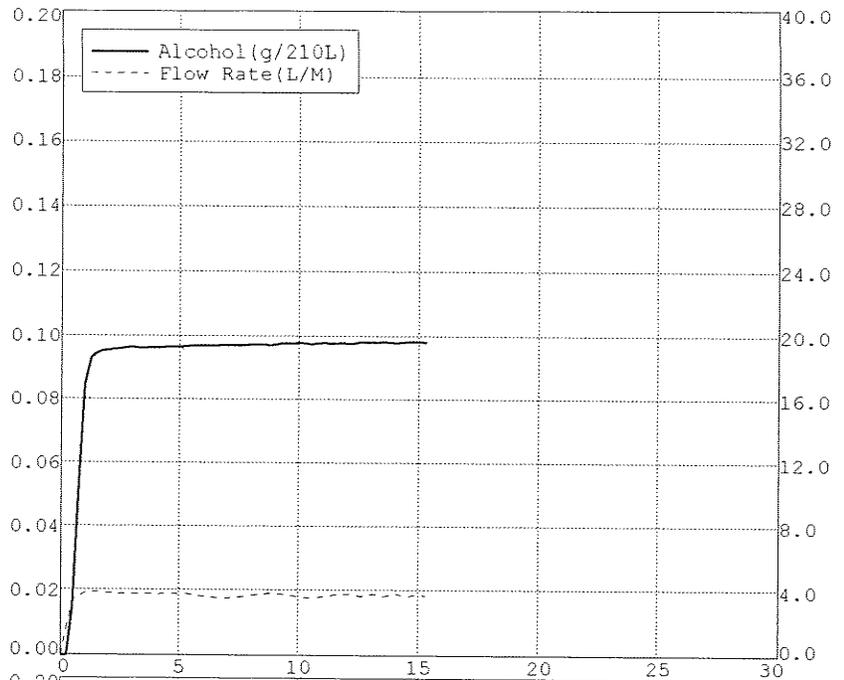

*Ch. B. Geisler #201*