

SUPERVISOR TEST




WARREN COUNTY  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 01/07/2021

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:08
INTERNAL STANDARD	VERIFIED	15:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:09
BLANK TEST	0.00	15:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:11
BLANK TEST	0.00	15:12

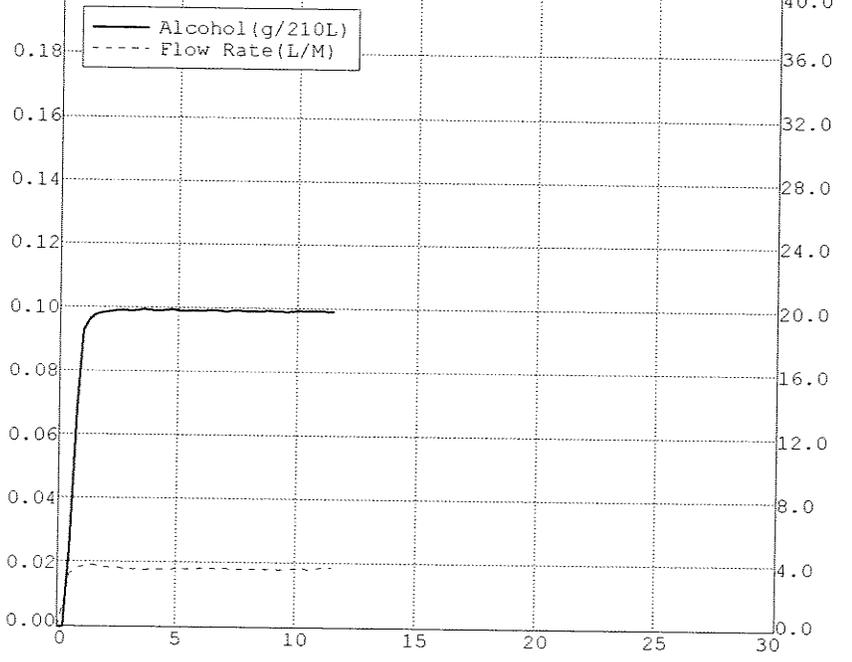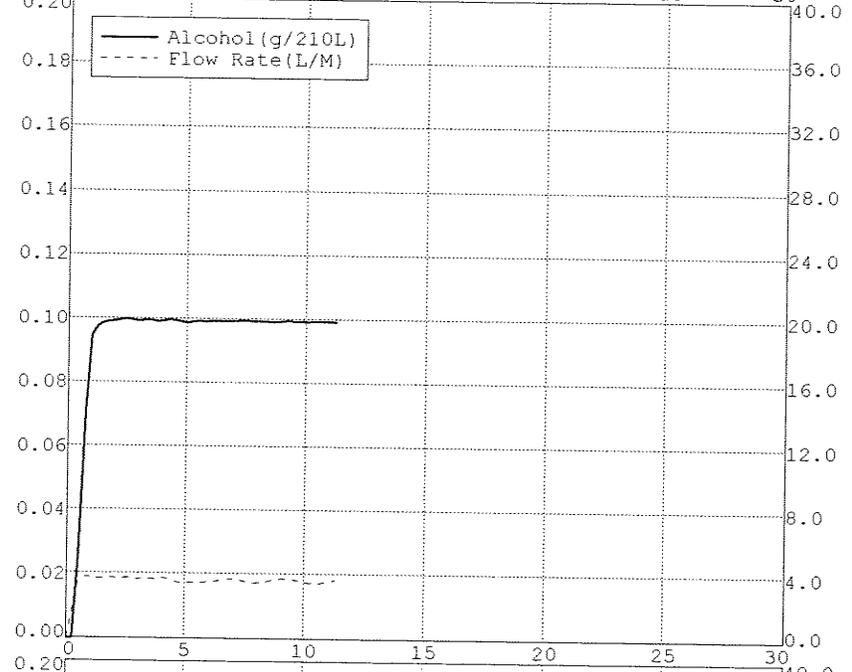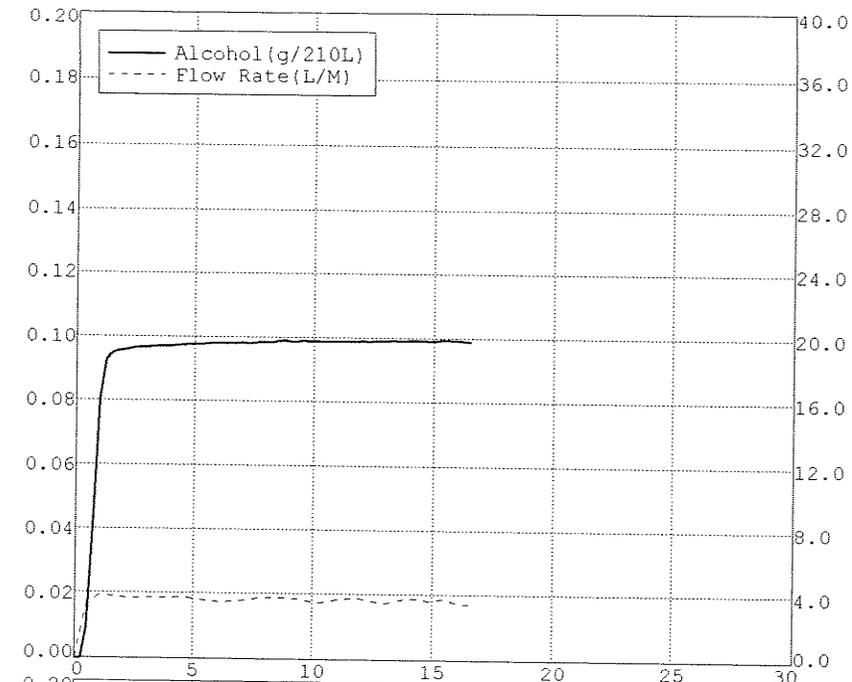

*Handwritten signature: C. B. Geisler #248*