

SUPERVISOR TEST




WARREN COUNTY  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 01/15/2021

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:31
INTERNAL STANDARD	VERIFIED	13:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:32
BLANK TEST	0.00	13:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:33
BLANK TEST	0.00	13:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:34
BLANK TEST	0.00	13:35

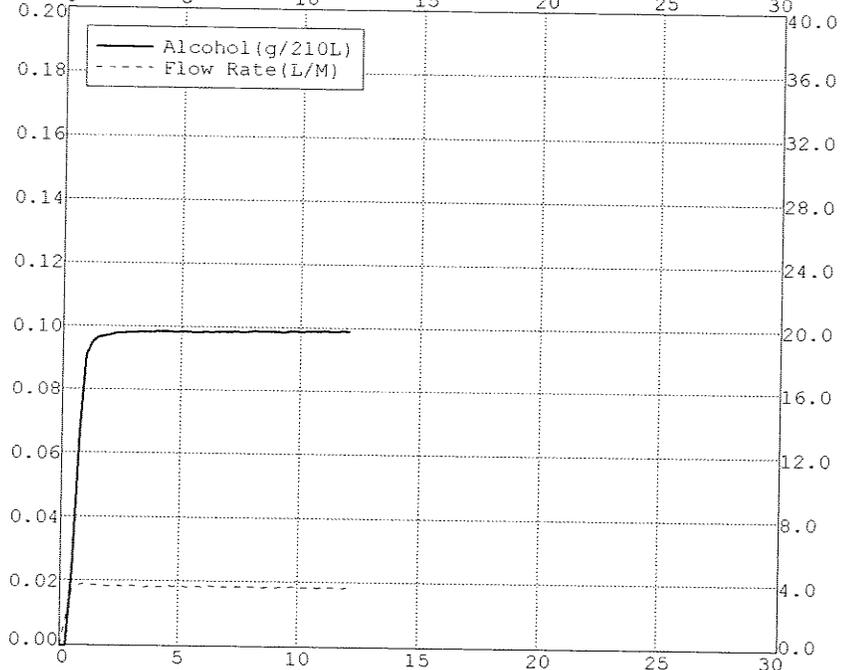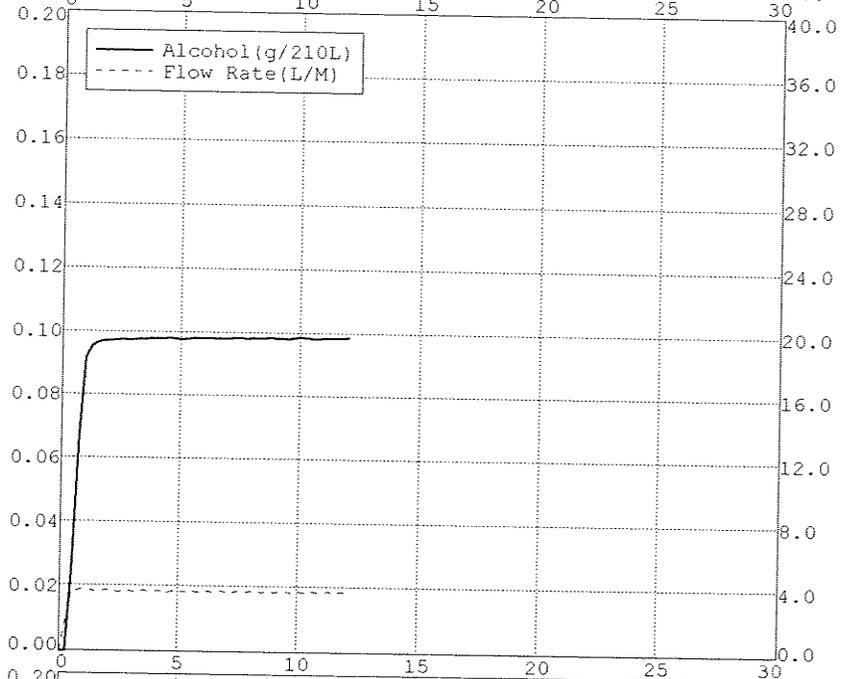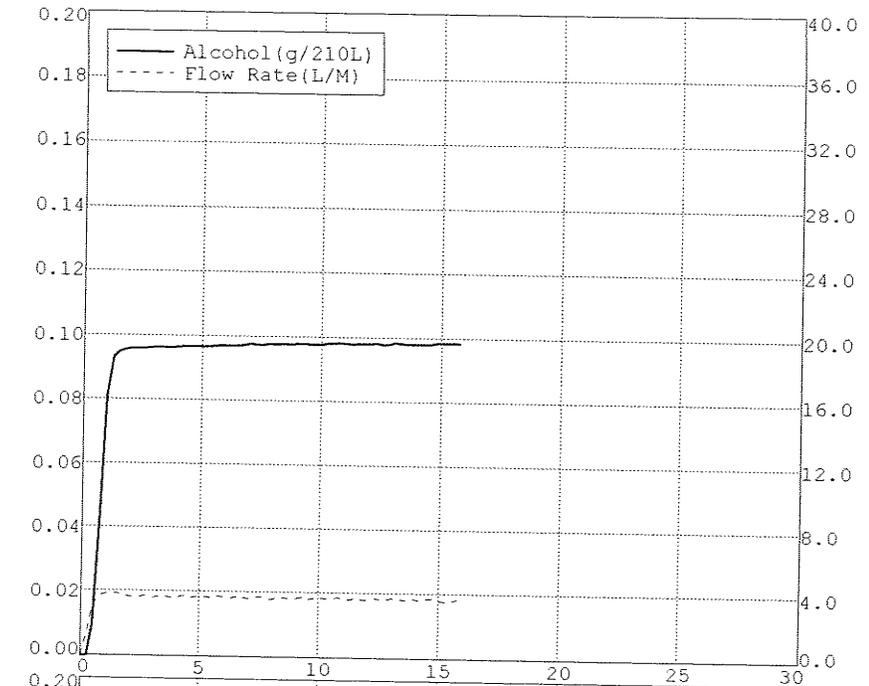

*Handwritten signature and initials:*  
 Sgt. Charles B. Geisler  
 #266