

SUPERVISOR TEST




WARREN COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 01/29/2021

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:40
INTERNAL STANDARD	VERIFIED	16:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:40
BLANK TEST	0.00	16:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:41
BLANK TEST	0.00	16:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:43
BLANK TEST	0.00	16:44

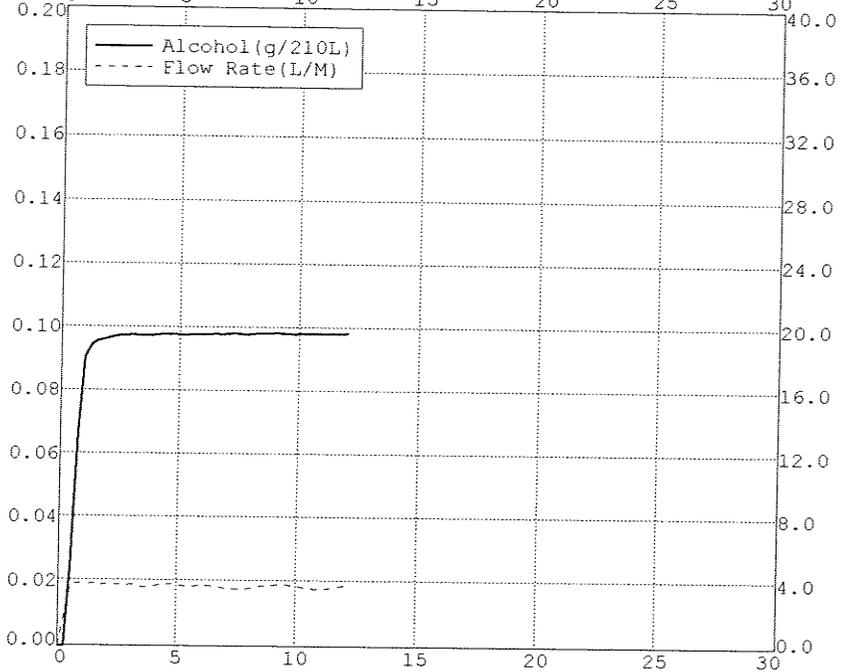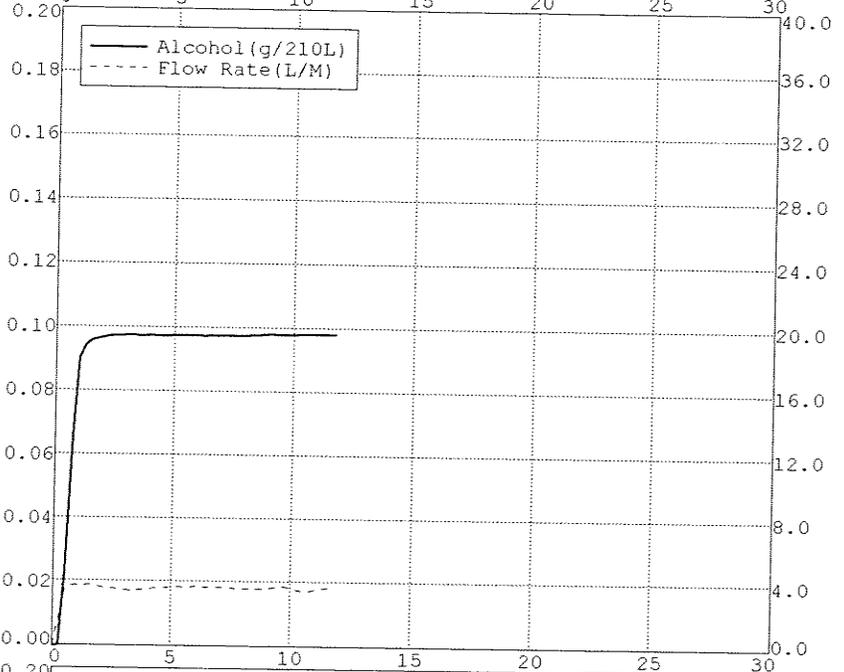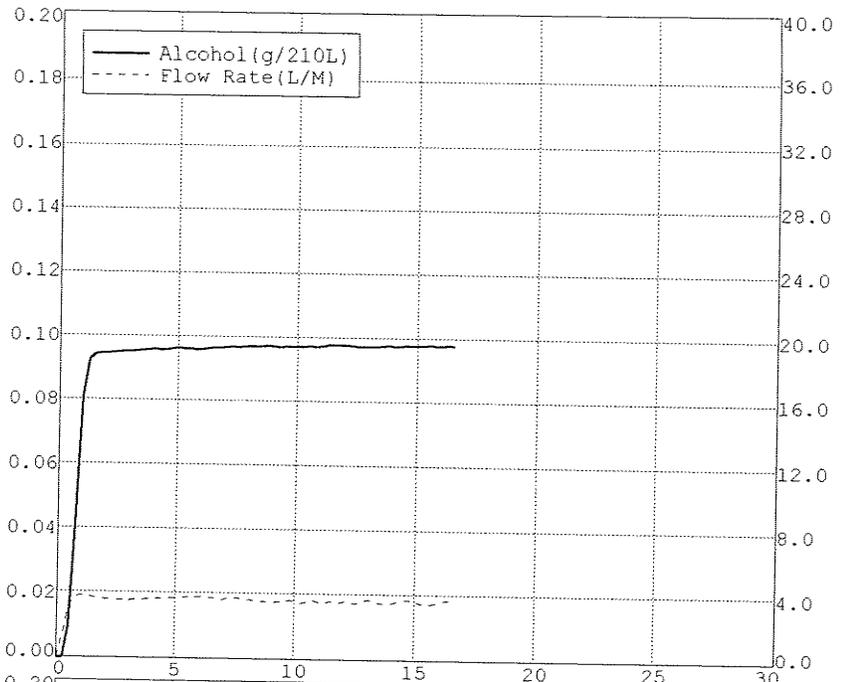

Charles B. Geisler #245