

SUPERVISOR TEST




WARREN COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 02/08/2021

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:29
INTERNAL STANDARD	VERIFIED	14:29
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:30
BLANK TEST	0.00	14:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:31
BLANK TEST	0.00	14:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:32
BLANK TEST	0.00	14:33

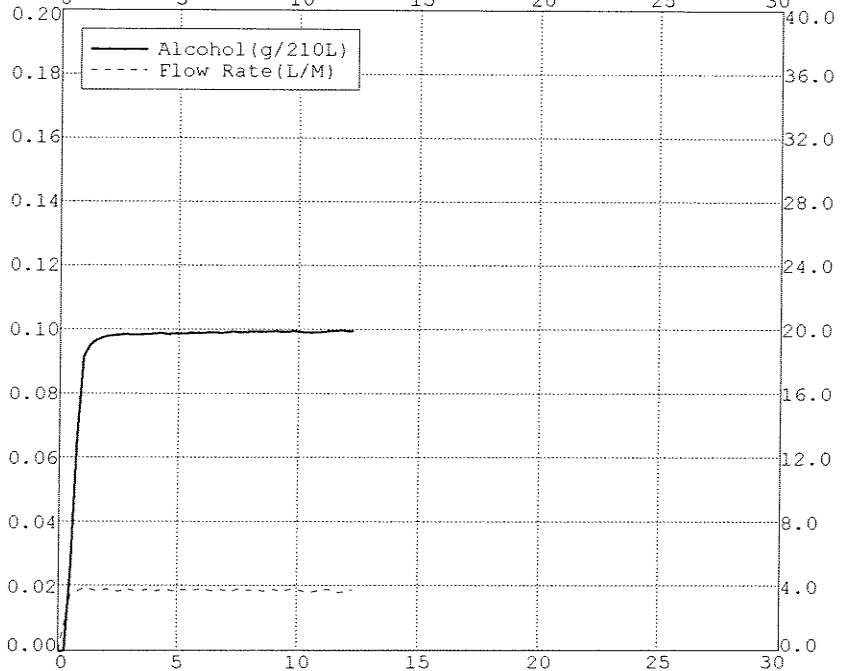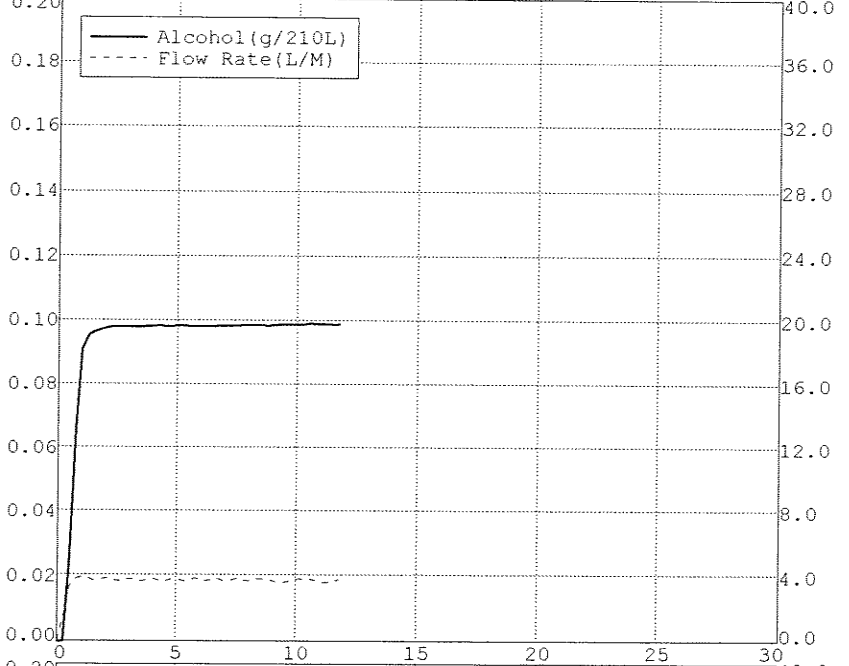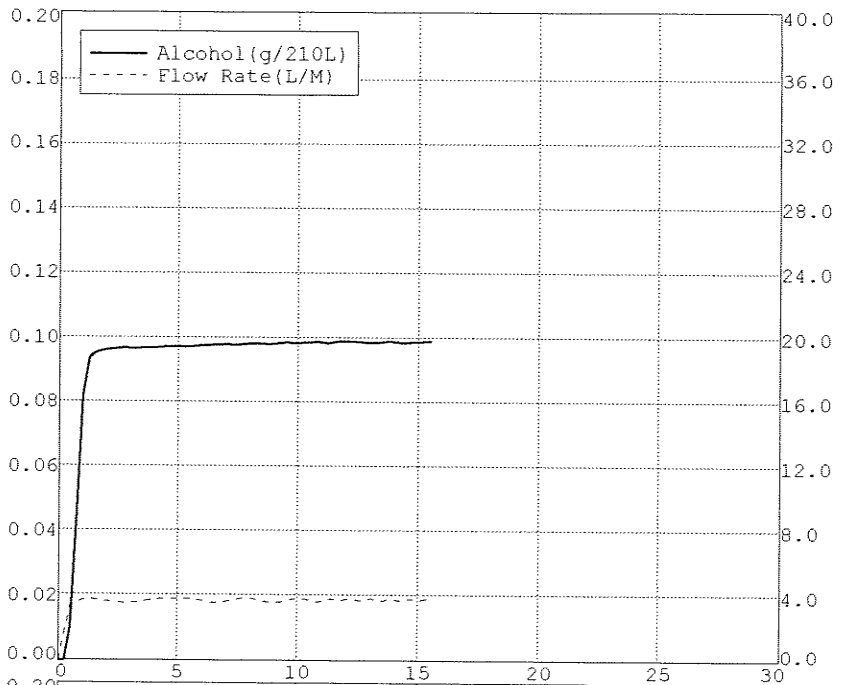

Charles B. Geisler