

SUPERVISOR TEST




WARREN COUNTY
 SHERIFF'S OFFICE
 DATAMASTER dmt: 144506

Date: 02/14/2021

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:19
INTERNAL STANDARD	VERIFIED	15:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:19
BLANK TEST	0.00	15:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:20
BLANK TEST	0.00	15:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:21
BLANK TEST	0.00	15:22

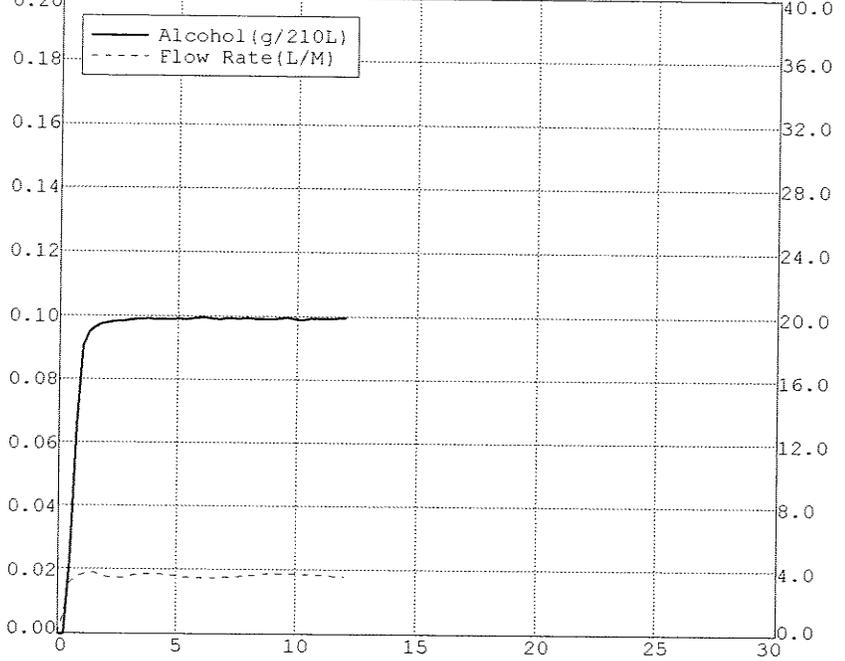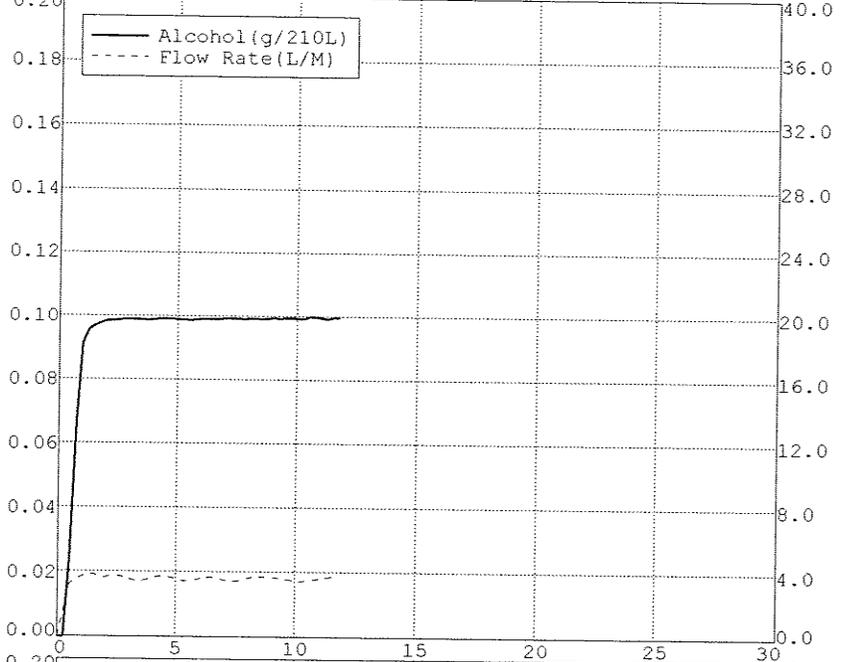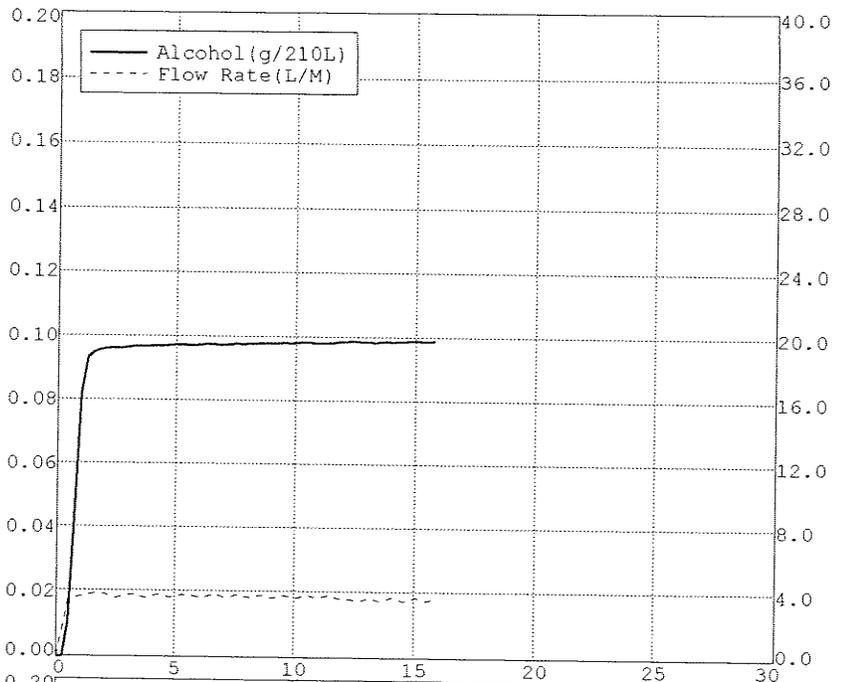

Sgt. Charles B. Geisler #201