

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 02/22/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:59
INTERNAL STANDARD	VERIFIED	11:59
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	12:00
BLANK TEST	0.00	12:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:01
BLANK TEST	0.00	12:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:02
BLANK TEST	0.00	12:03

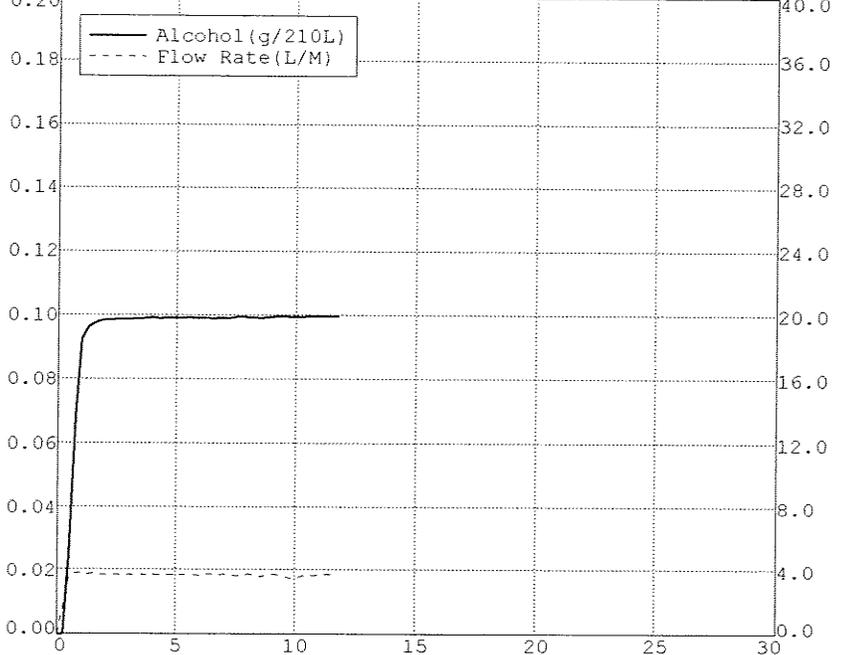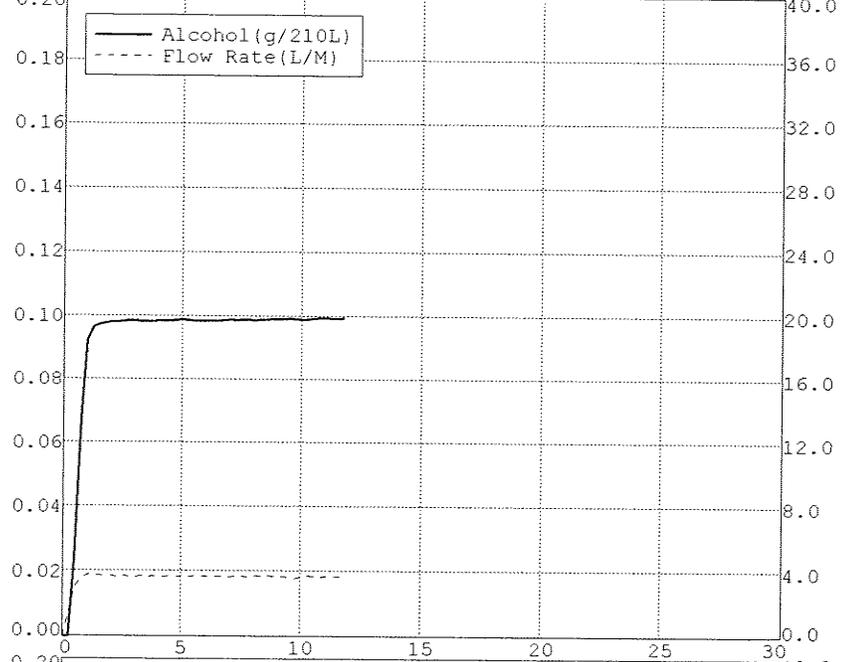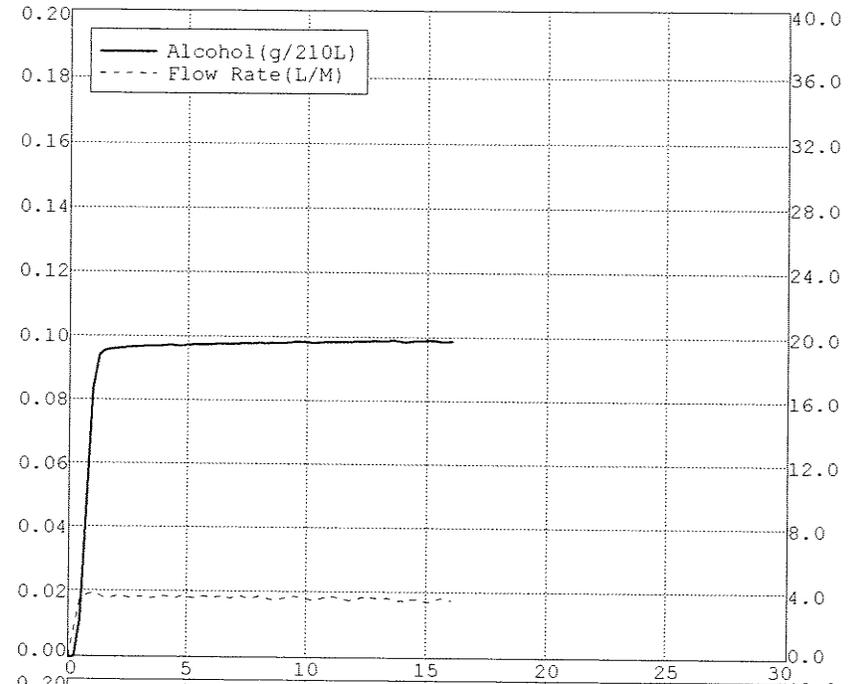

*Charles B Geisler* #248