

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 03/14/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:43
INTERNAL STANDARD	VERIFIED	13:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:44
BLANK TEST	0.00	13:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:45
BLANK TEST	0.00	13:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	13:46
BLANK TEST	0.00	13:47

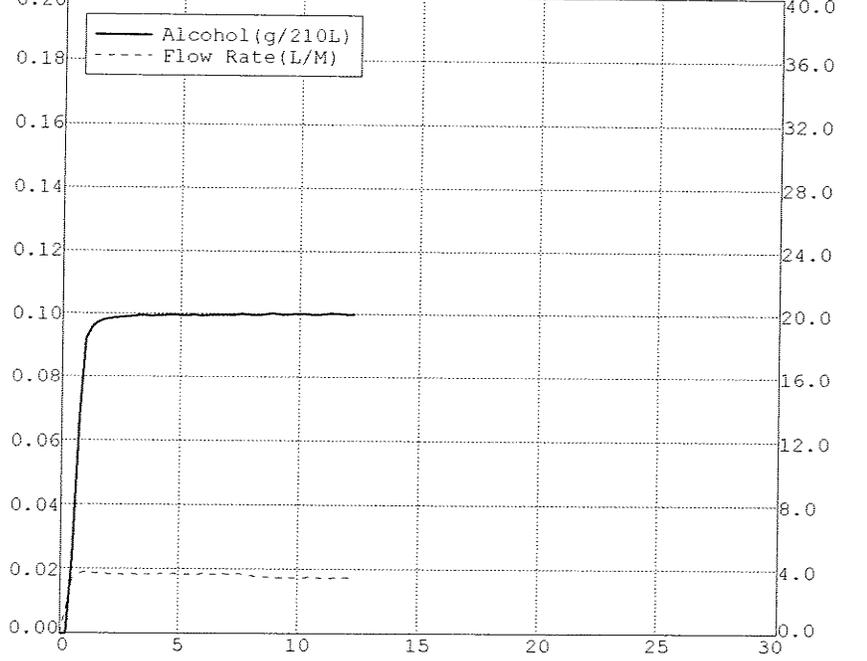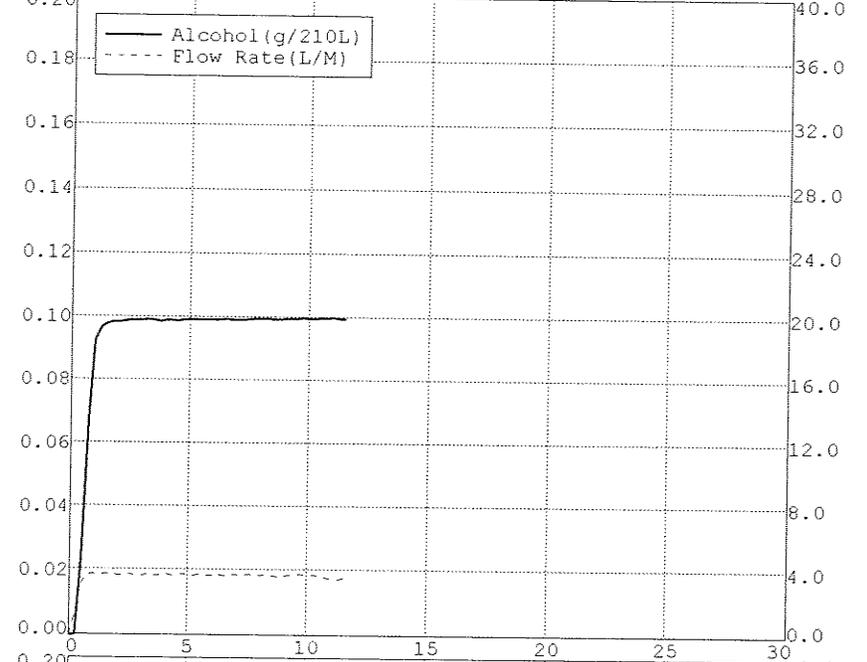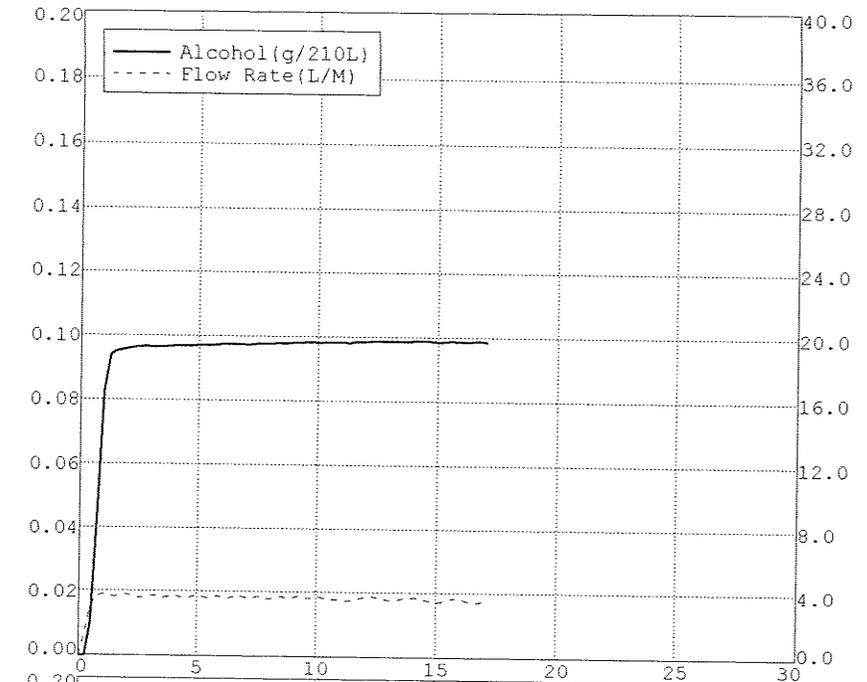

*Sgt. Charles B. Geisler #241*