

SUPERVISOR TEST



WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 03/28/2021

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20500

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:30
INTERNAL STANDARD	VERIFIED	14:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:31
BLANK TEST	0.00	14:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:32
BLANK TEST	0.00	14:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:33
BLANK TEST	0.00	14:34

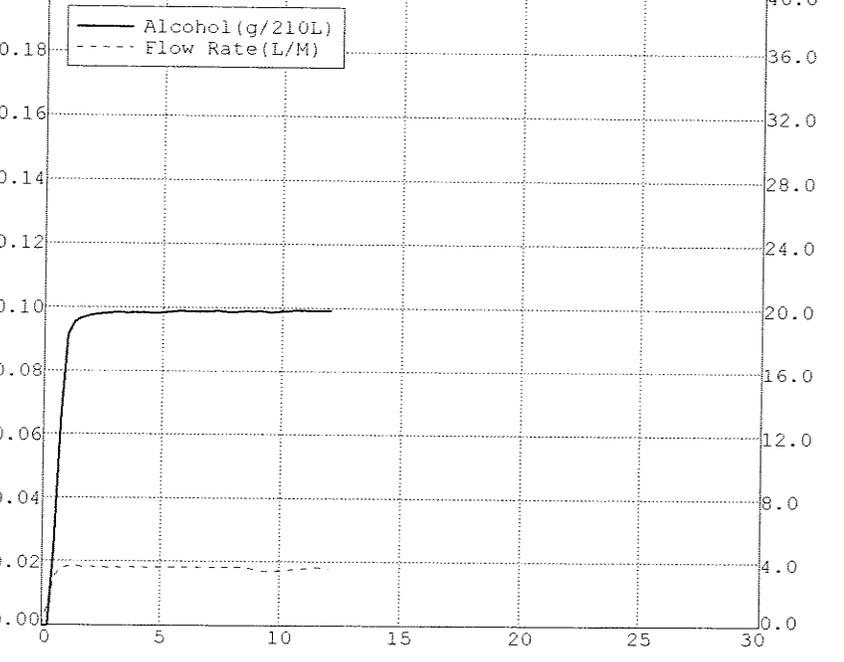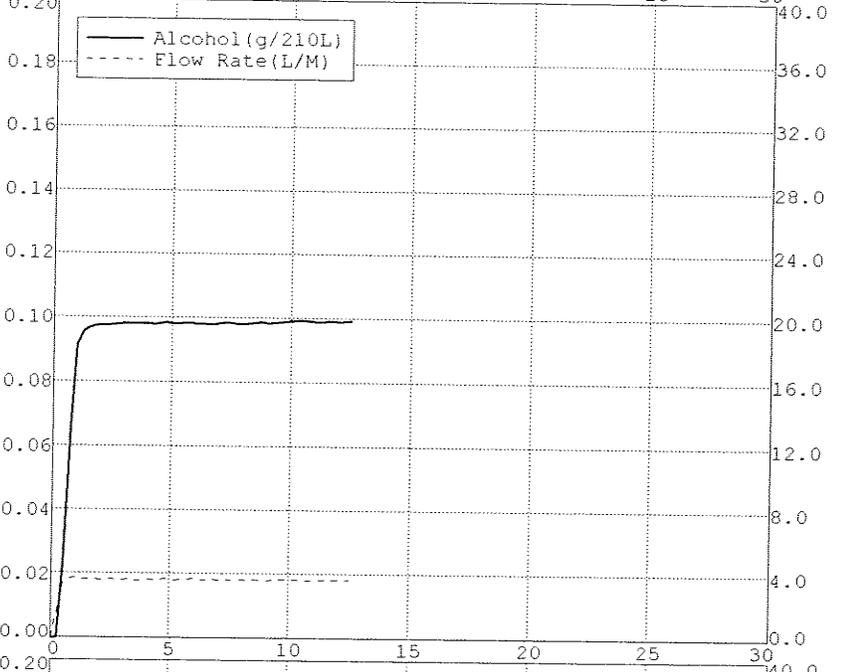

*Signature*  
#241