

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 04/11/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:18
INTERNAL STANDARD	VERIFIED	16:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:18
BLANK TEST	0.00	16:19
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:20
BLANK TEST	0.00	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:21
BLANK TEST	0.00	16:22

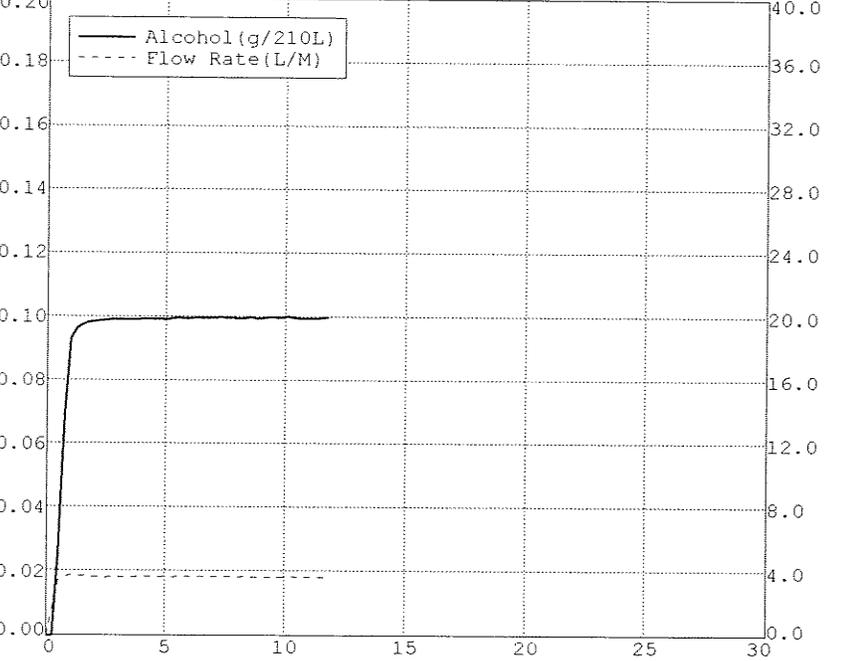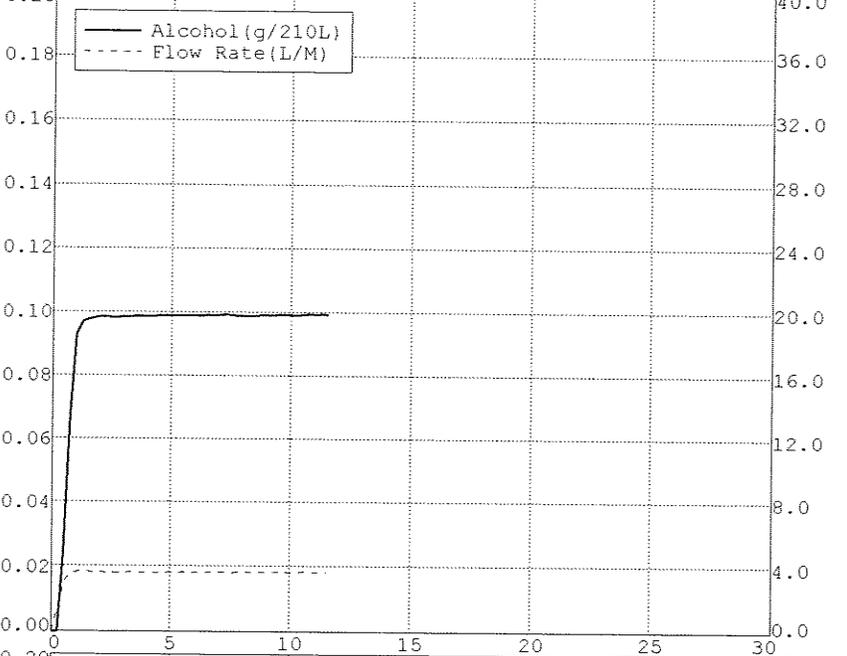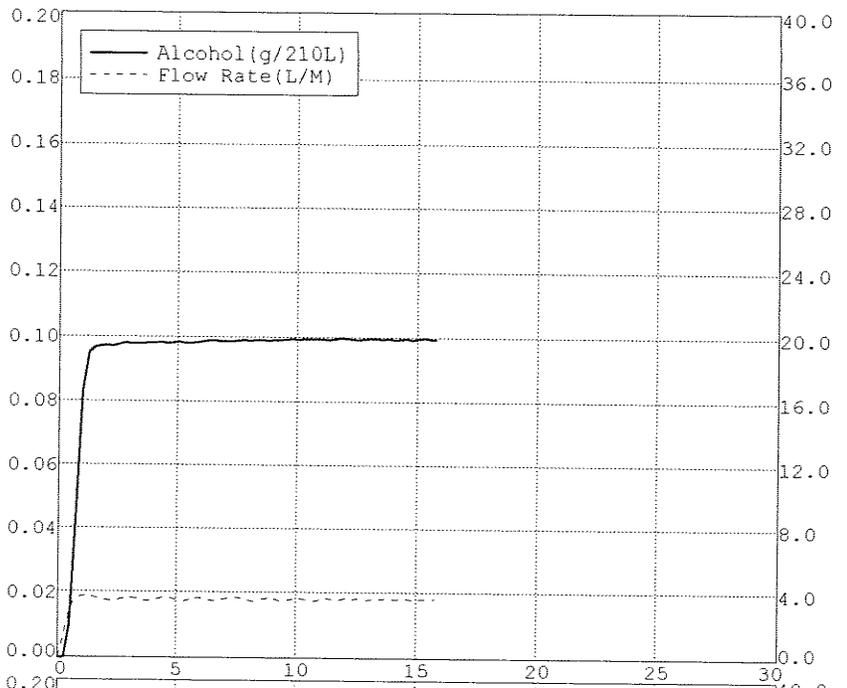

Charles B. Geisler #291