

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 05/23/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21020

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:21
INTERNAL STANDARD	VERIFIED	14:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:22
BLANK TEST	0.00	14:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:23
BLANK TEST	0.00	14:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:24
BLANK TEST	0.00	14:25

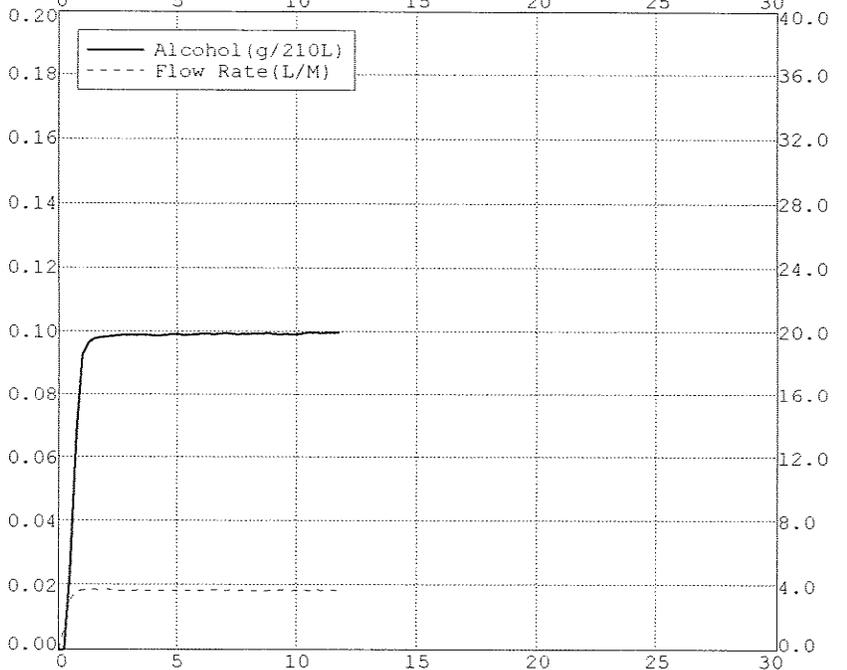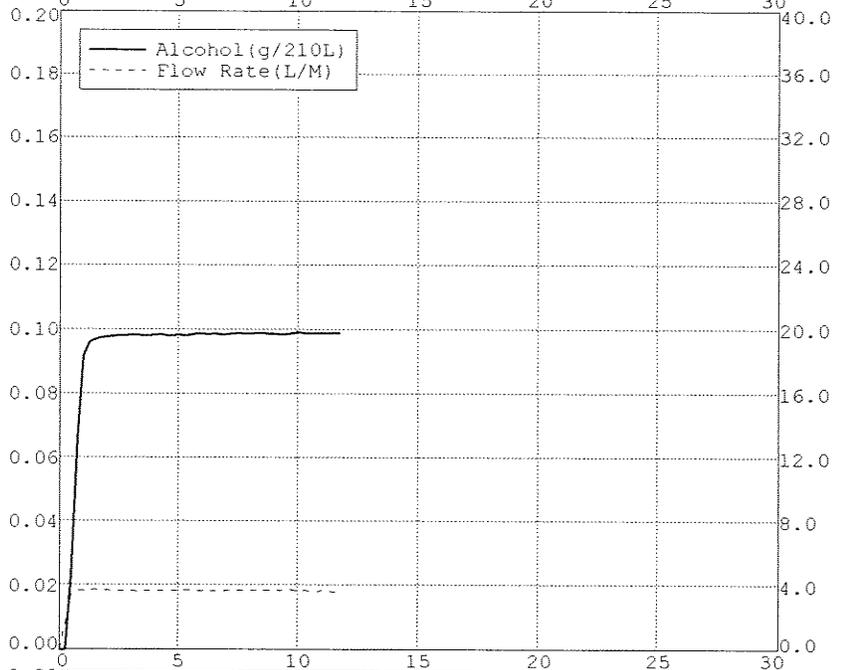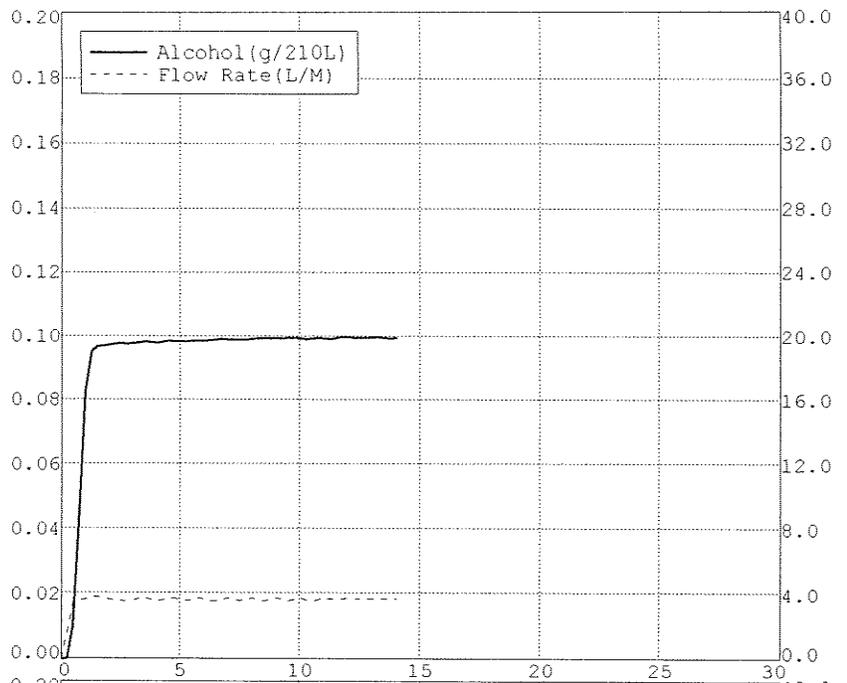

Sgt. Charles B. Geisler #224