

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 06/01/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:19
INTERNAL STANDARD	VERIFIED	14:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:19
BLANK TEST	0.00	14:20
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:21
BLANK TEST	0.00	14:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:22
BLANK TEST	0.00	14:23

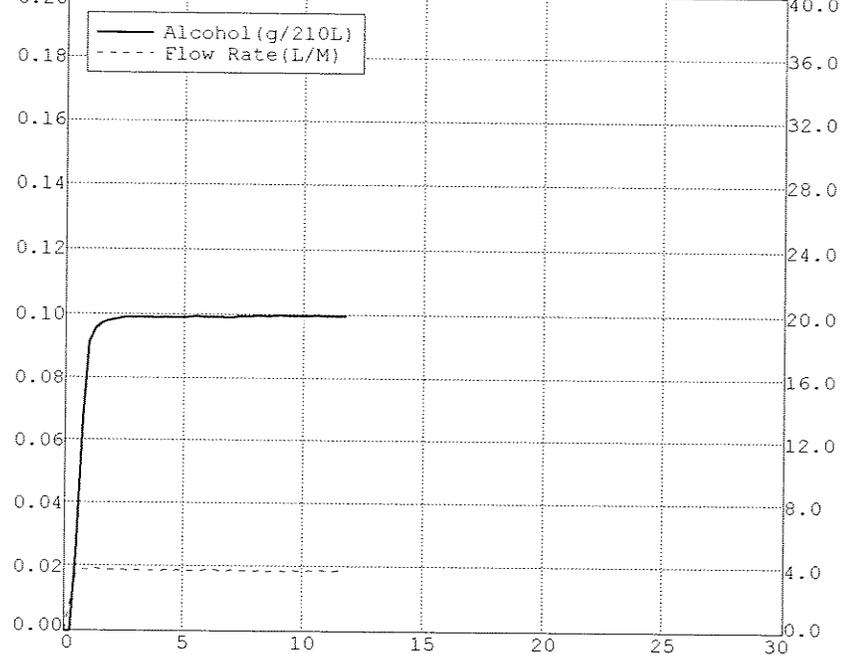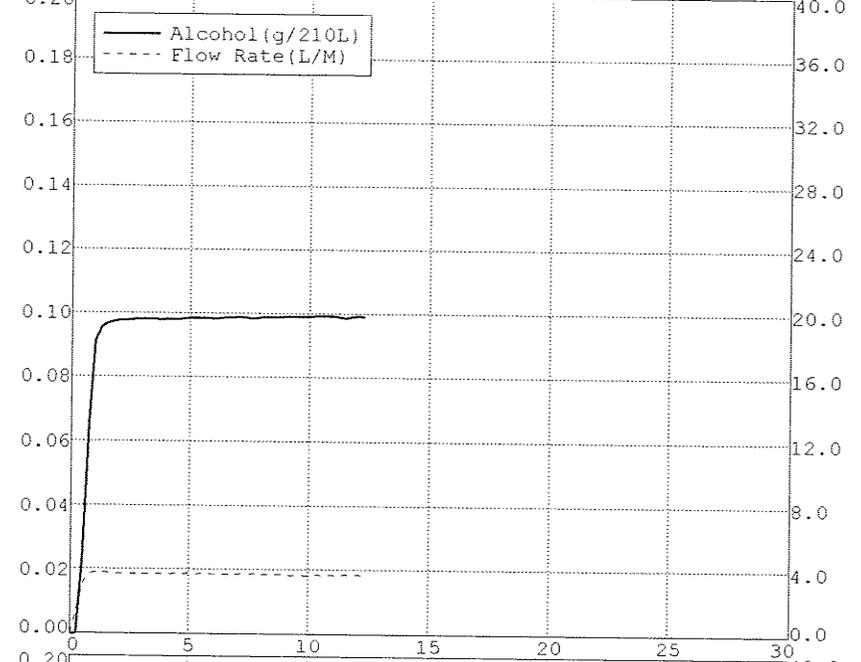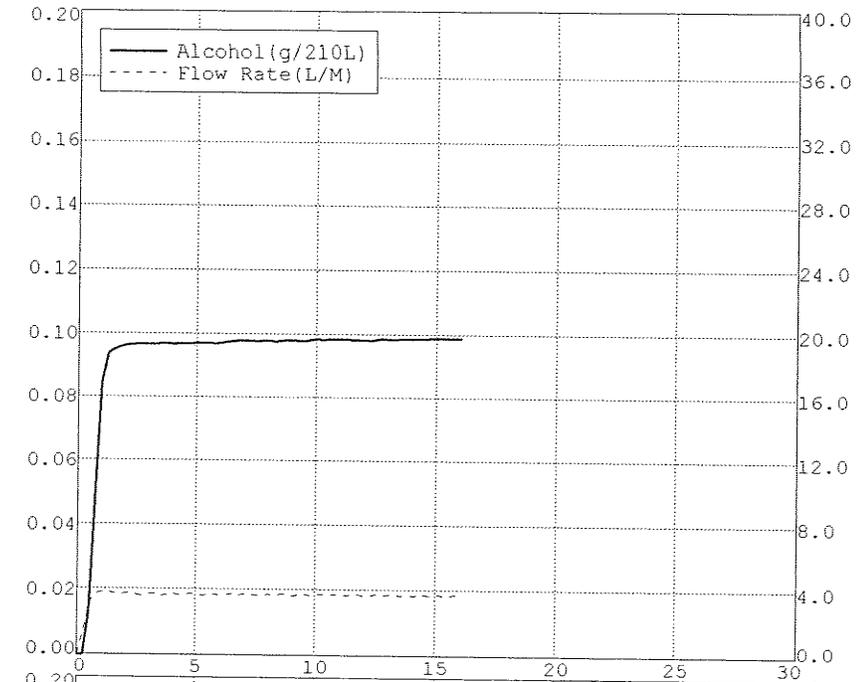

Handwritten signature: C. B. Geisler #244