

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 06/06/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:10
INTERNAL STANDARD	VERIFIED	10:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	10:10
BLANK TEST	0.00	10:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:11
BLANK TEST	0.00	10:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	10:13
BLANK TEST	0.00	10:14

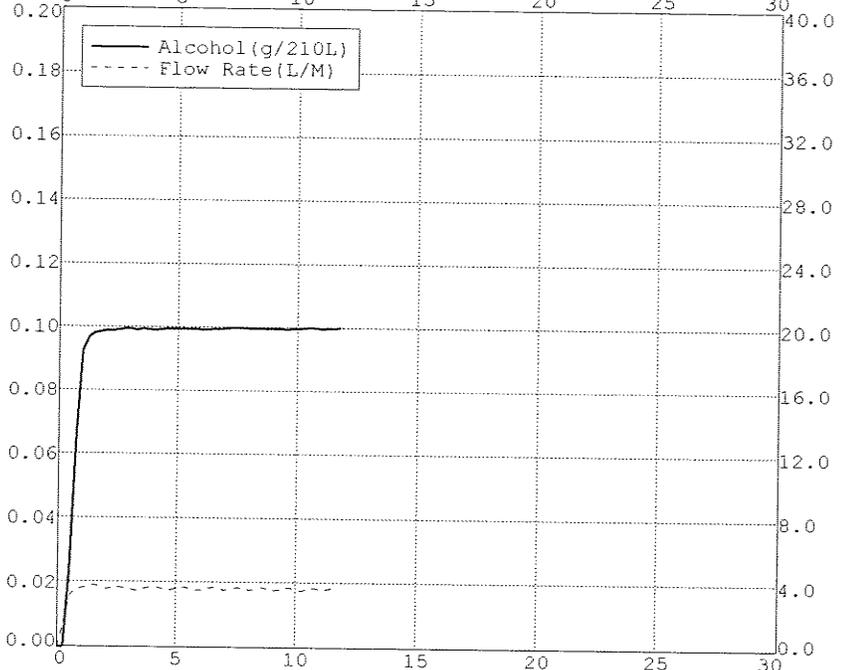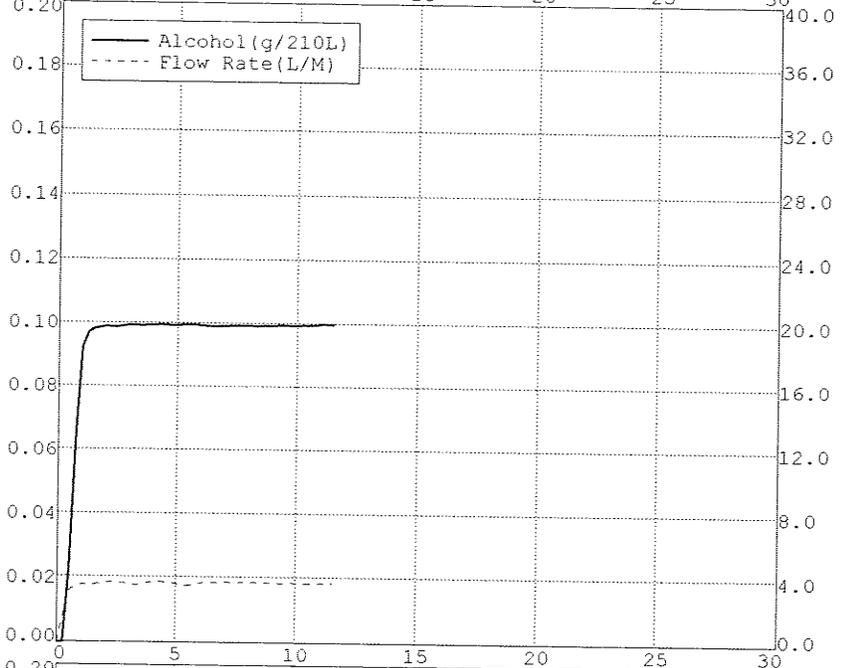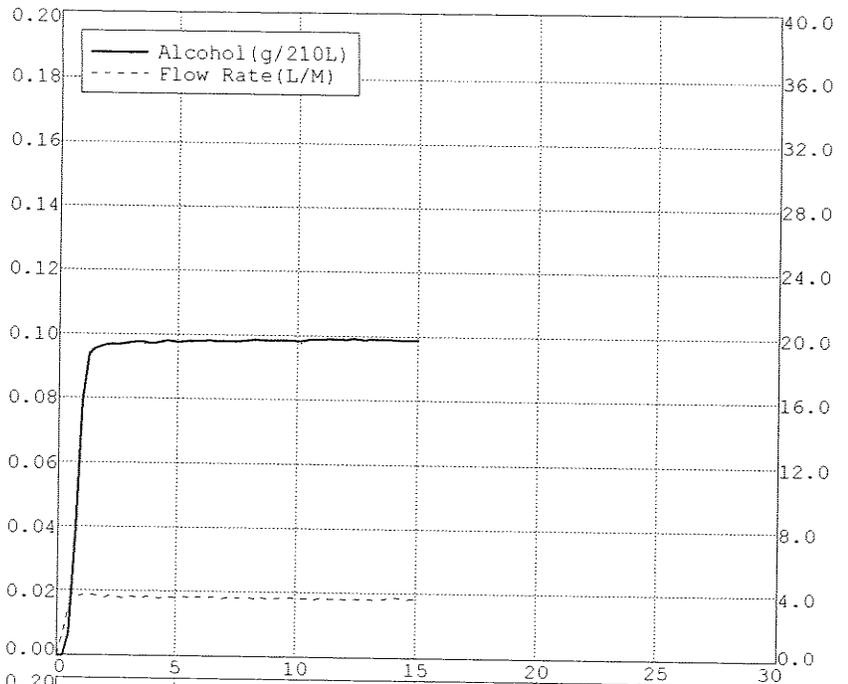

Handwritten signature and initials
#201