

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 06/14/2021

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21100

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:39
INTERNAL STANDARD	VERIFIED	16:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:40
BLANK TEST	0.00	16:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	16:41
BLANK TEST	0.00	16:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:42
BLANK TEST	0.00	16:43

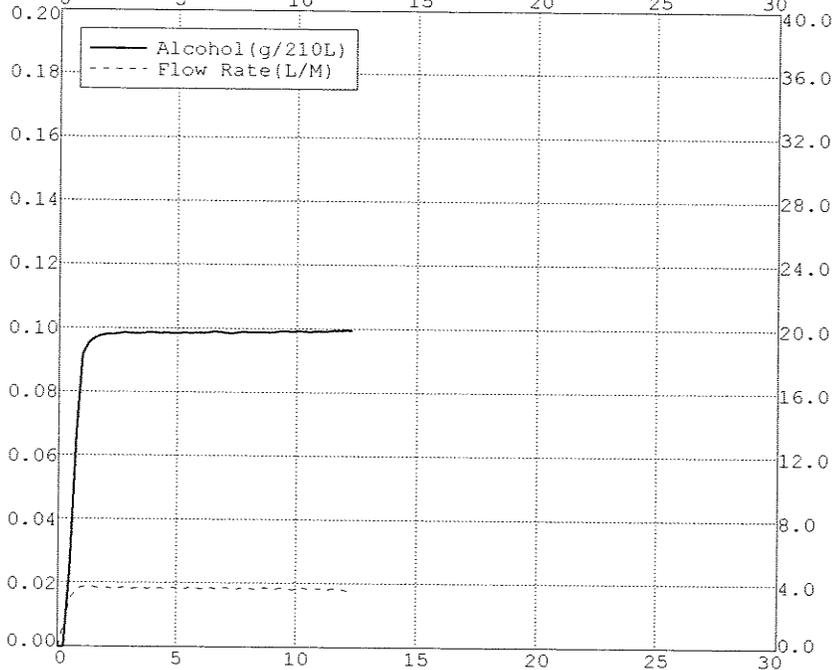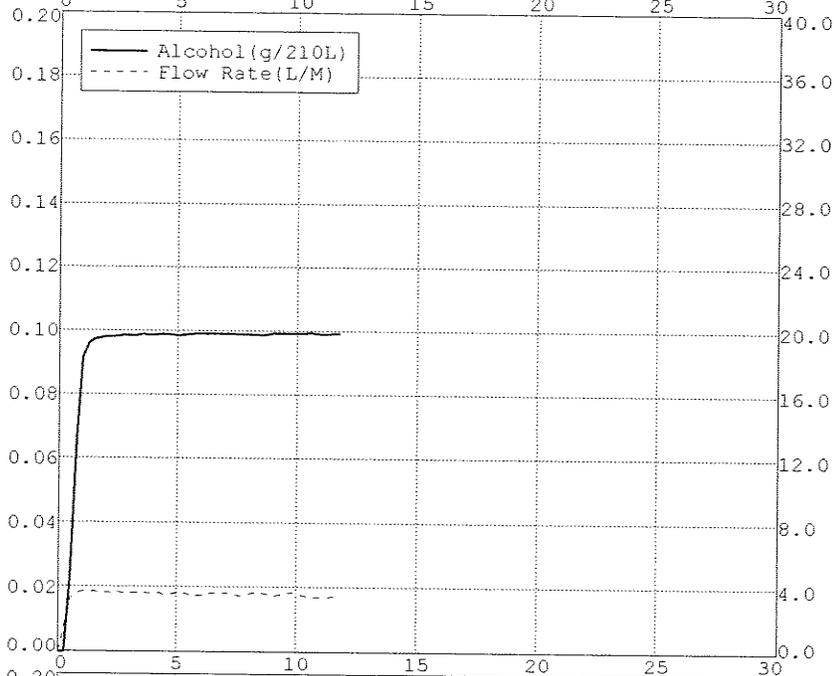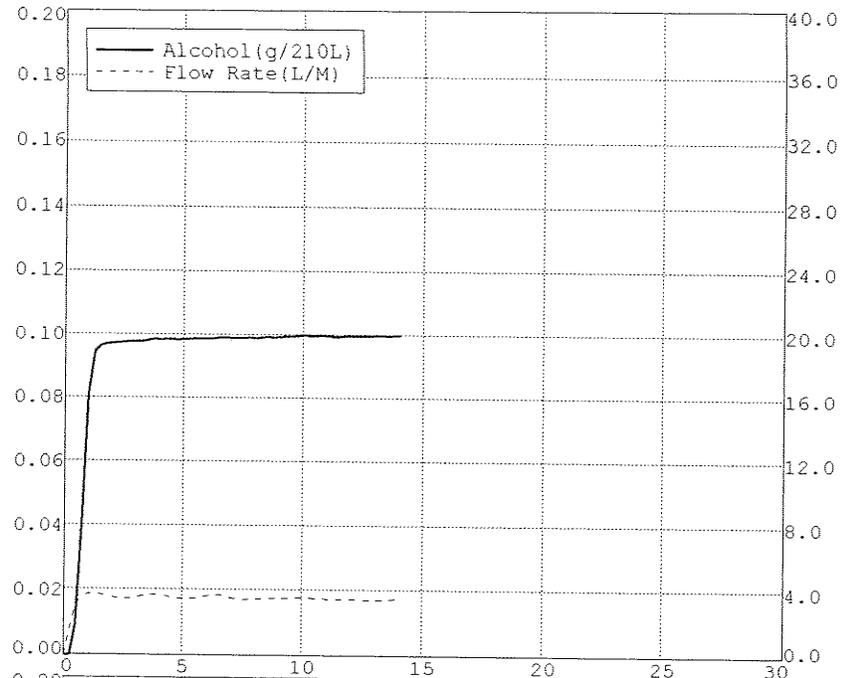

Handwritten signatures and initials:
J. M. B. [Signature] #241