

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/16/2022

OPERATOR NAME:  
SEAN T SMITH  
Permit #: 46227  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:13
INTERNAL STANDARD	VERIFIED	11:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:13
BLANK TEST	0.00	11:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	11:15
BLANK TEST	0.00	11:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	11:16
BLANK TEST	0.00	11:17

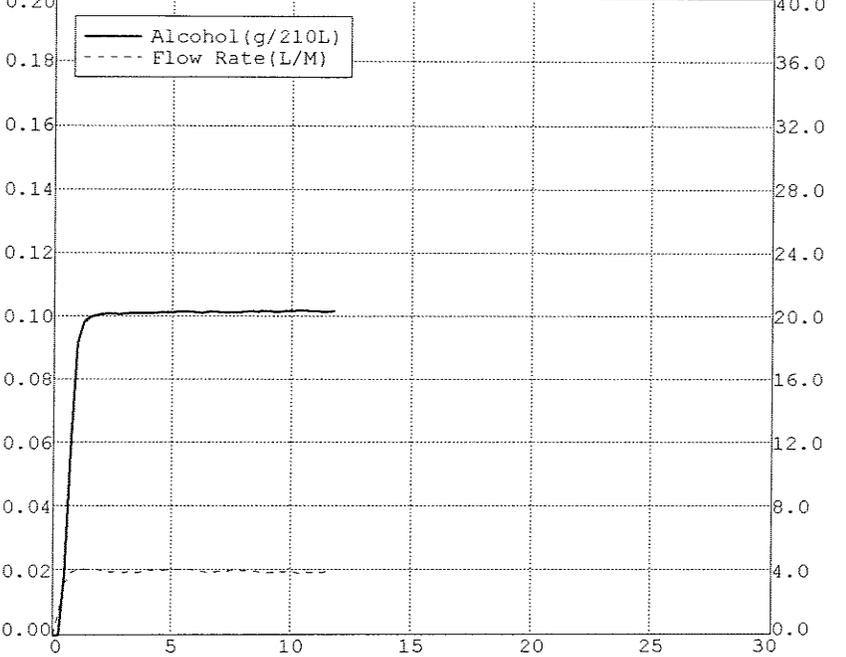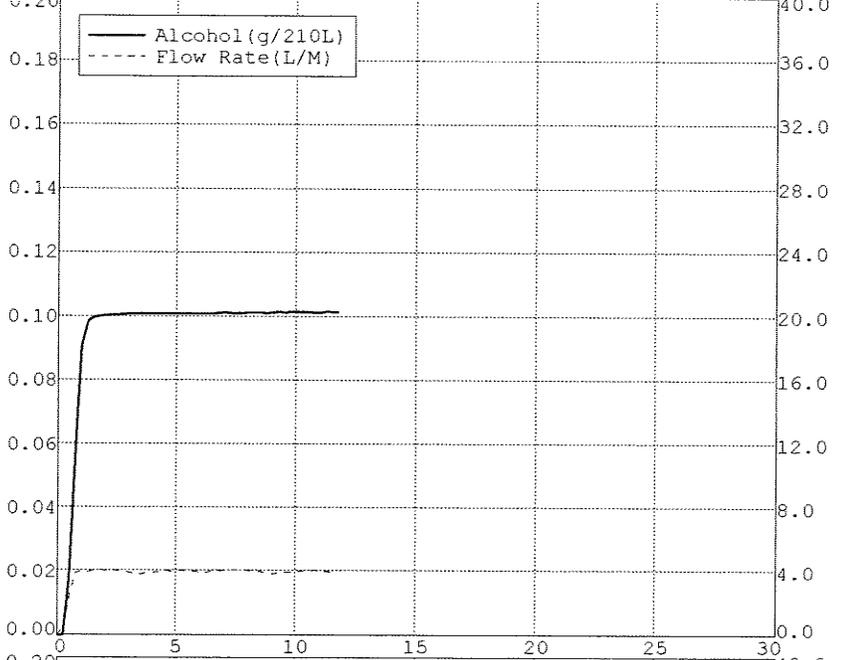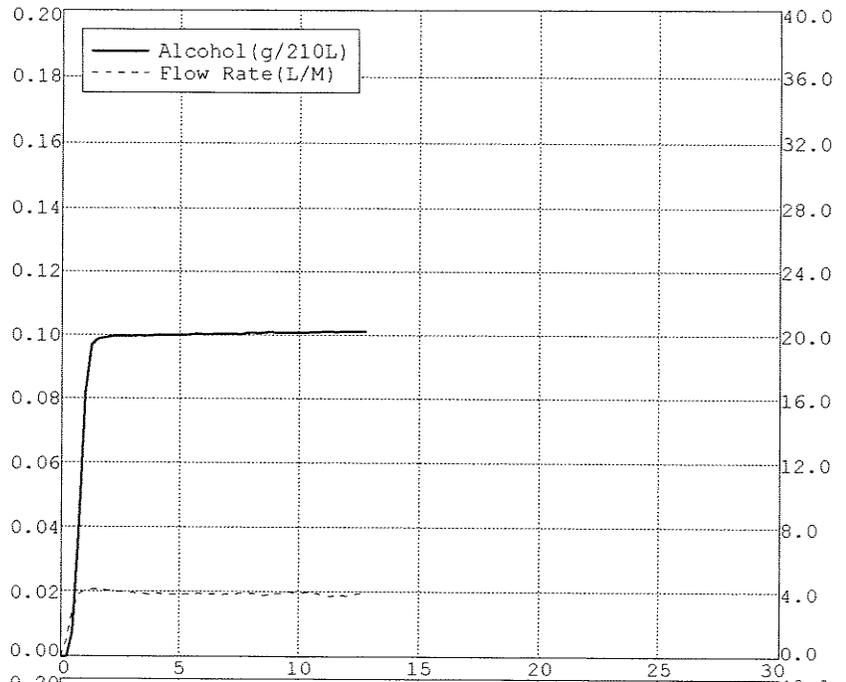

*Handwritten signature and initials*