

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 02/23/2022

OPERATOR NAME:
JAMES RIEHL
Permit #: 47503
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:05
INTERNAL STANDARD	VERIFIED	18:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:06
BLANK TEST	0.00	18:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:07
BLANK TEST	0.00	18:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:08
BLANK TEST	0.00	18:09

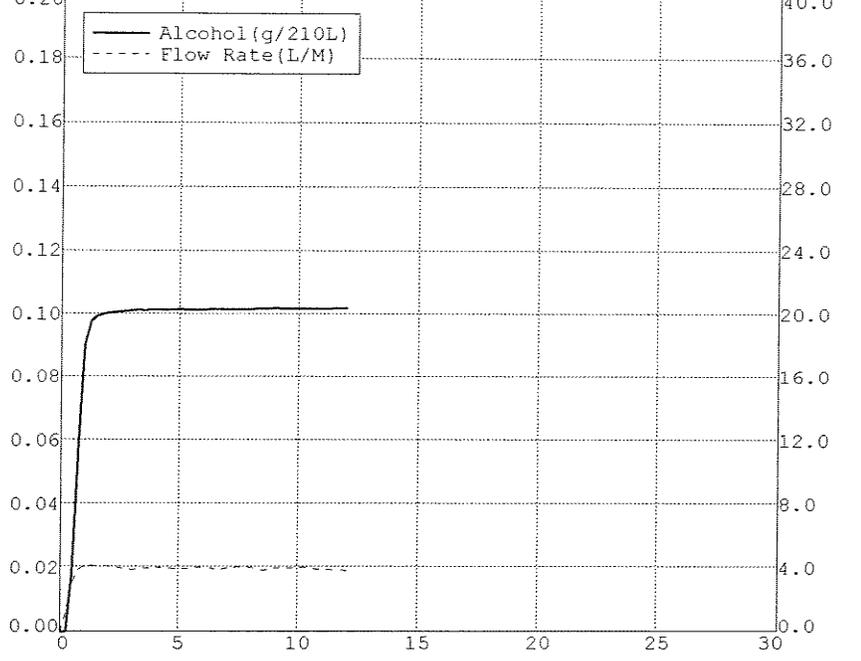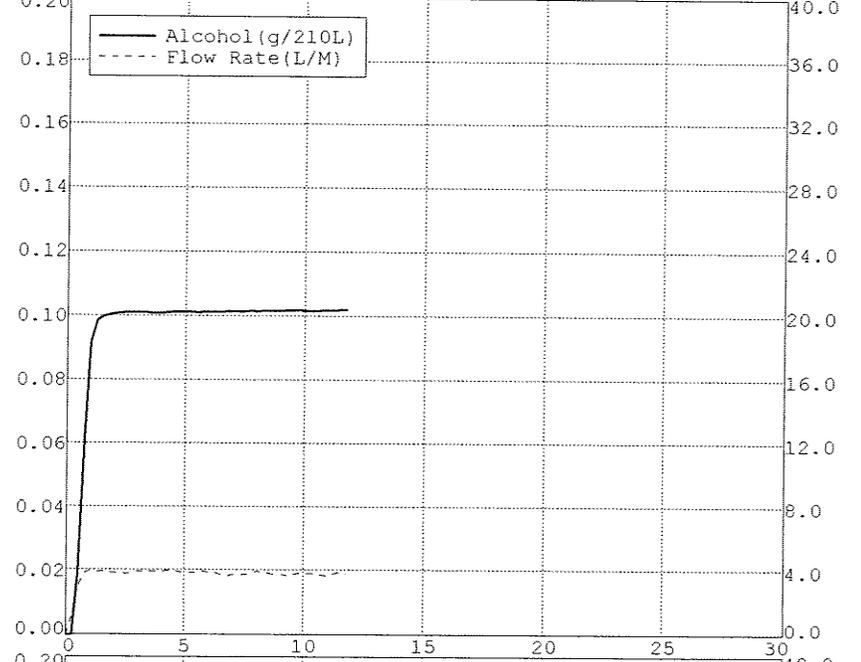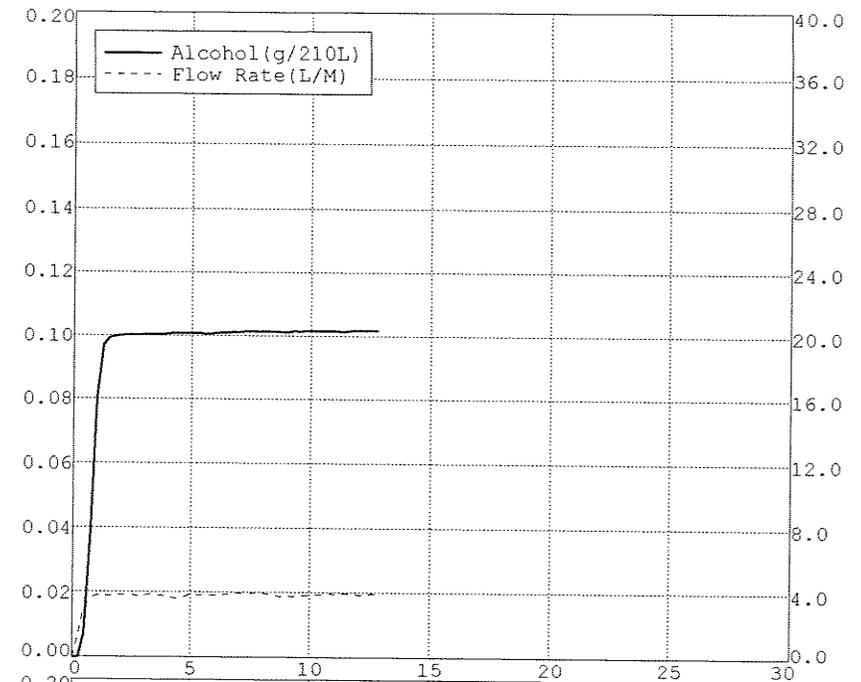

#820