

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 03/23/2022

OPERATOR NAME:
 J T COON
 Permit #: 36043
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 21440

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:16
INTERNAL STANDARD	VERIFIED	02:17
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:17
BLANK TEST	0.00	02:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:18
BLANK TEST	0.00	02:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:19
BLANK TEST	0.00	02:20

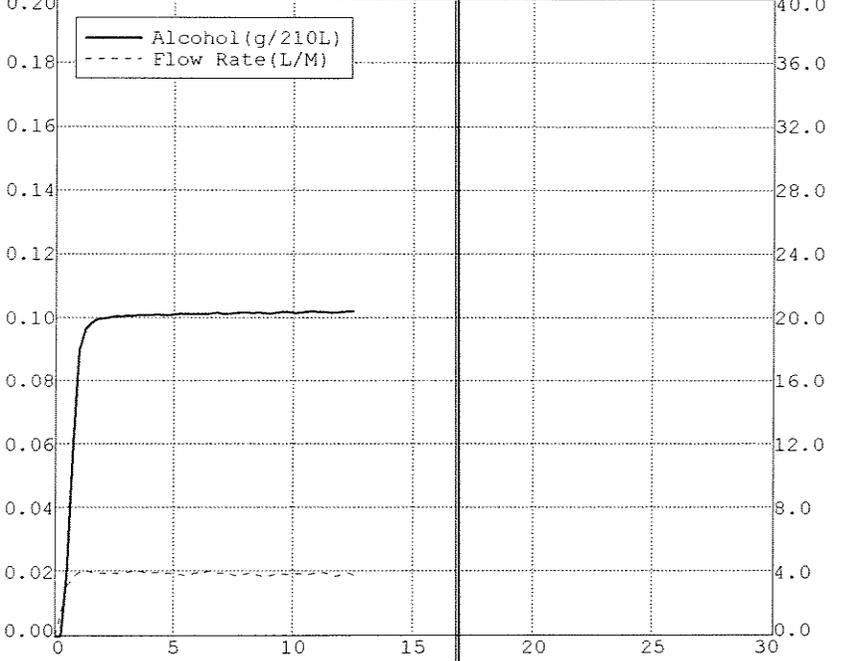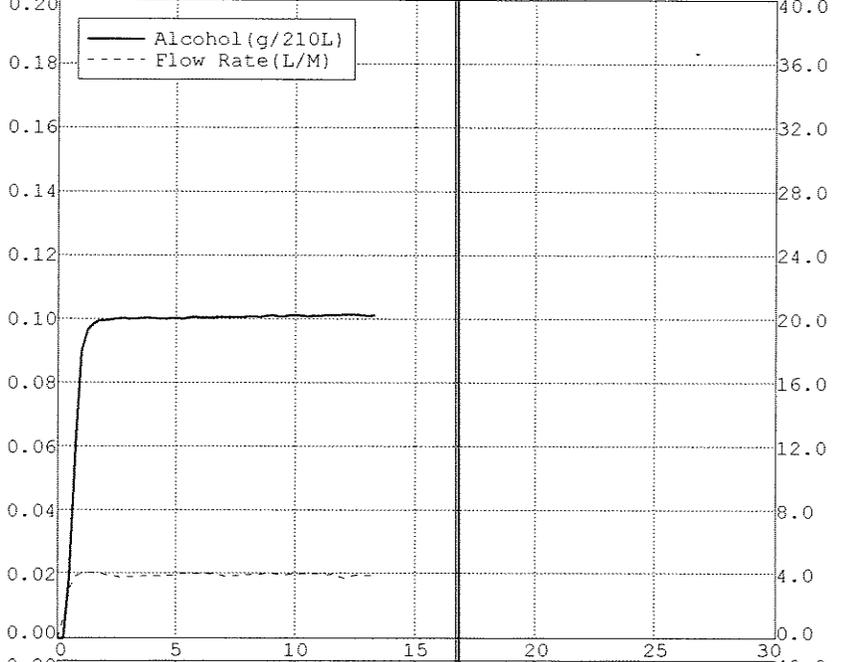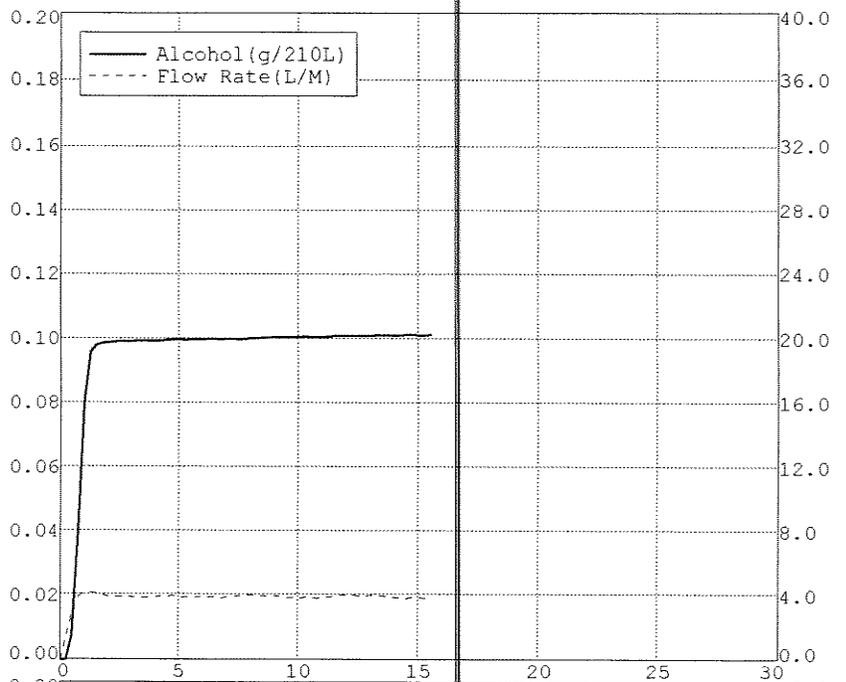

P.O. [Signature]
 341