

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/08/2022

OPERATOR NAME:
SEAN T SMITH
Permit #: 46227
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22030

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:47
INTERNAL STANDARD	VERIFIED	15:47
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:48
BLANK TEST	0.00	15:49
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:49
BLANK TEST	0.00	15:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:50
BLANK TEST	0.00	15:51

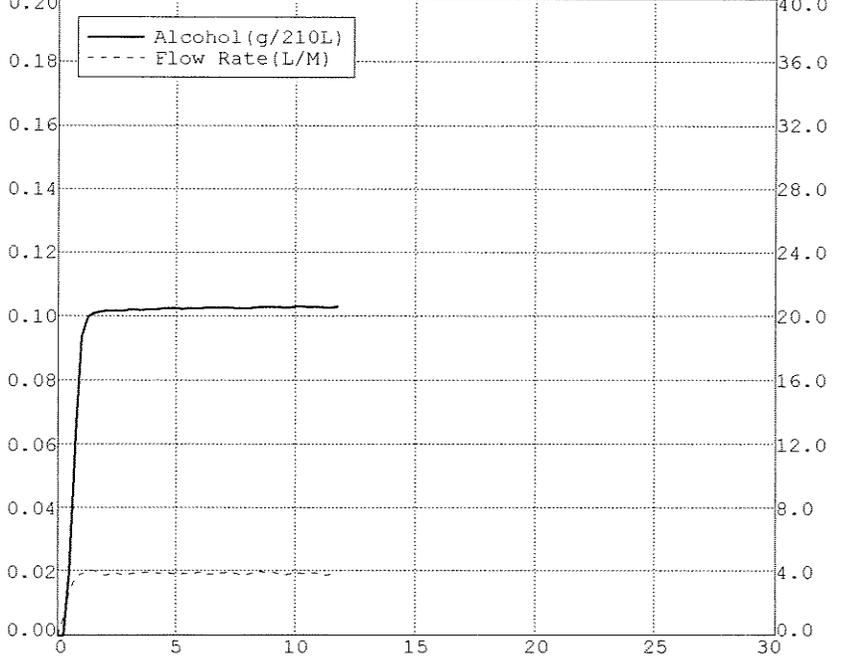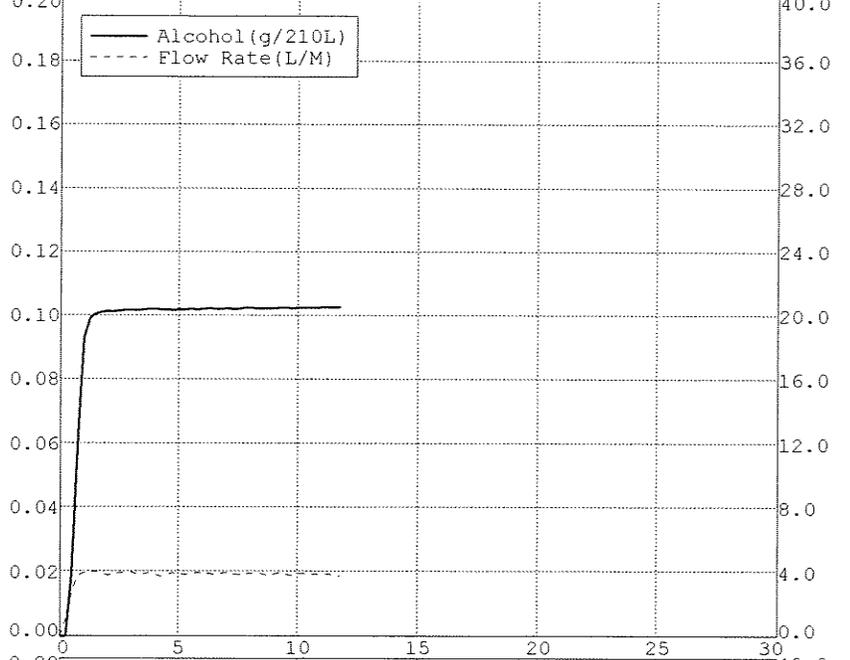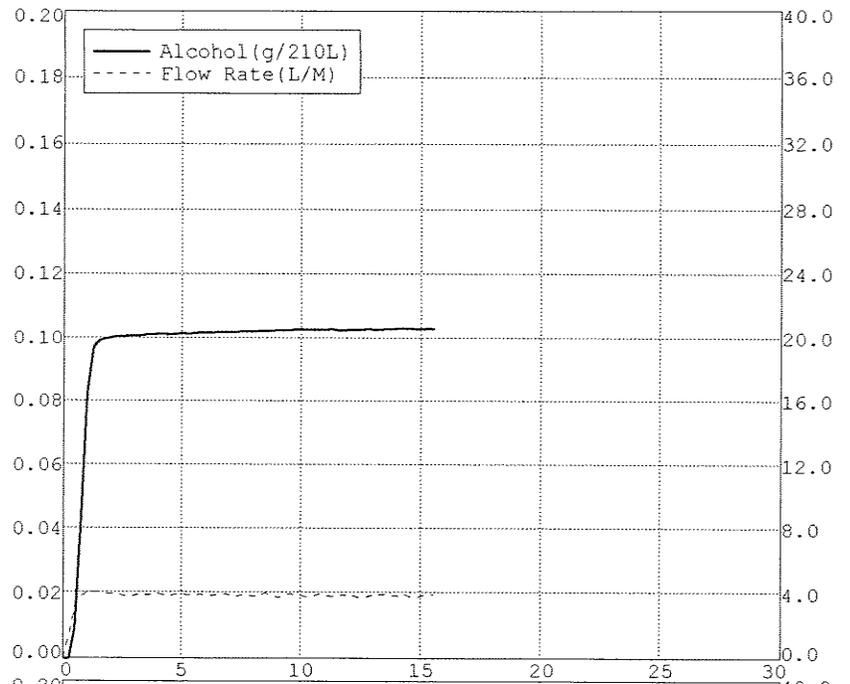

Handwritten signature