

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 06/01/2022

OPERATOR NAME:  
J RIEHL  
Permit #: 47503  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:16
INTERNAL STANDARD	VERIFIED	02:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:17
BLANK TEST	0.00	02:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:18
BLANK TEST	0.00	02:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:19
BLANK TEST	0.00	02:20

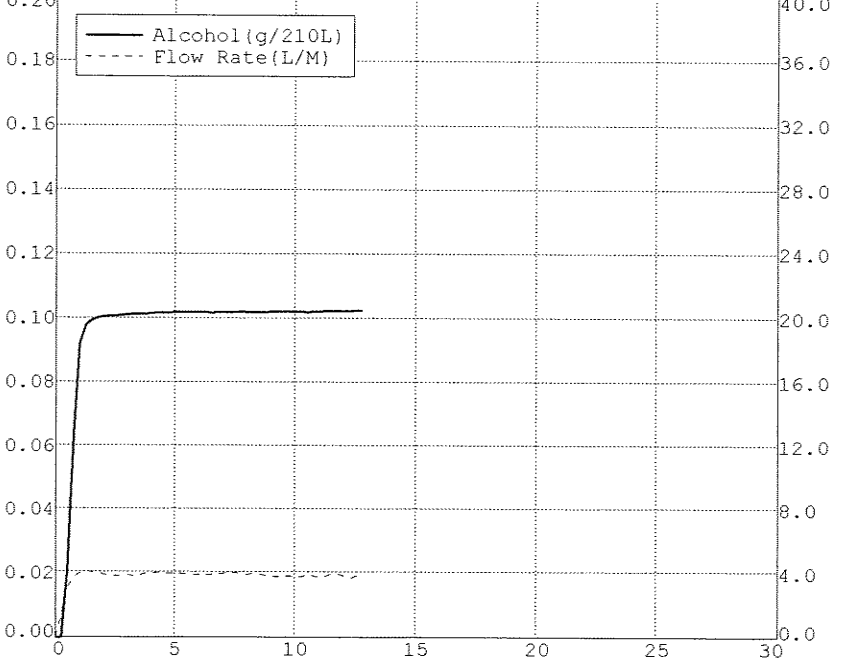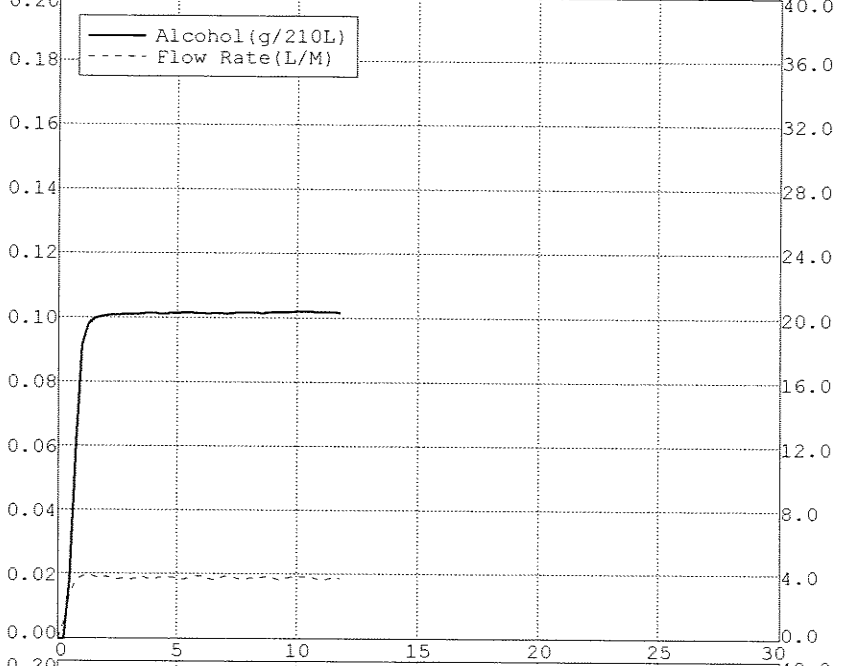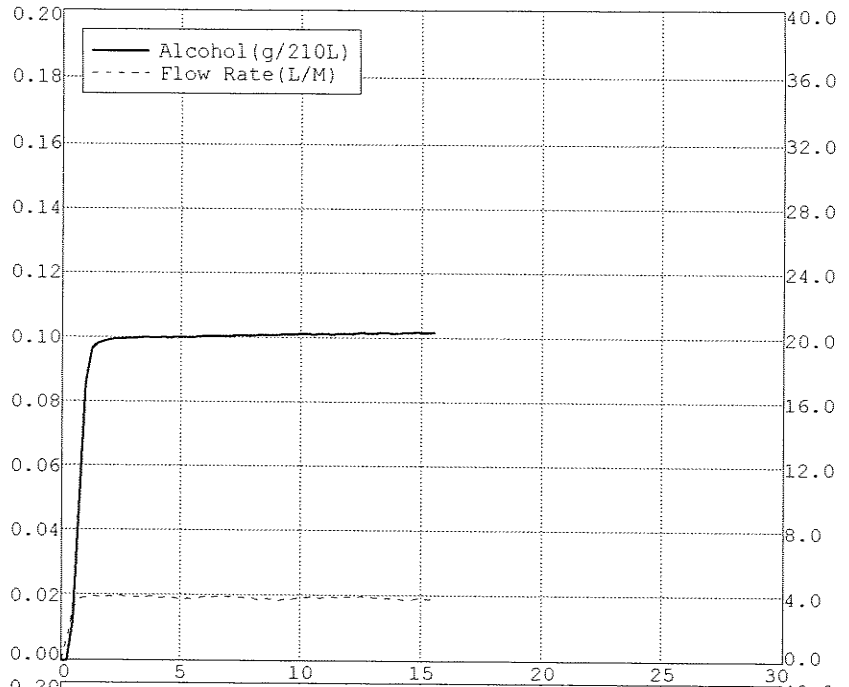

*#820*