

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/22/2022

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:51
INTERNAL STANDARD	VERIFIED	00:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:52
BLANK TEST	0.00	00:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:53
BLANK TEST	0.00	00:54
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:54
BLANK TEST	0.00	00:55

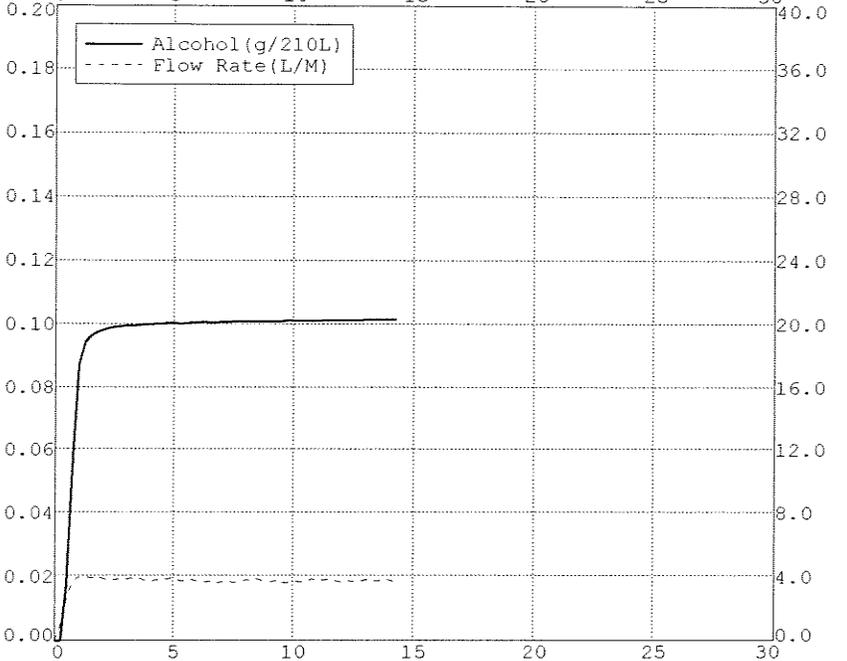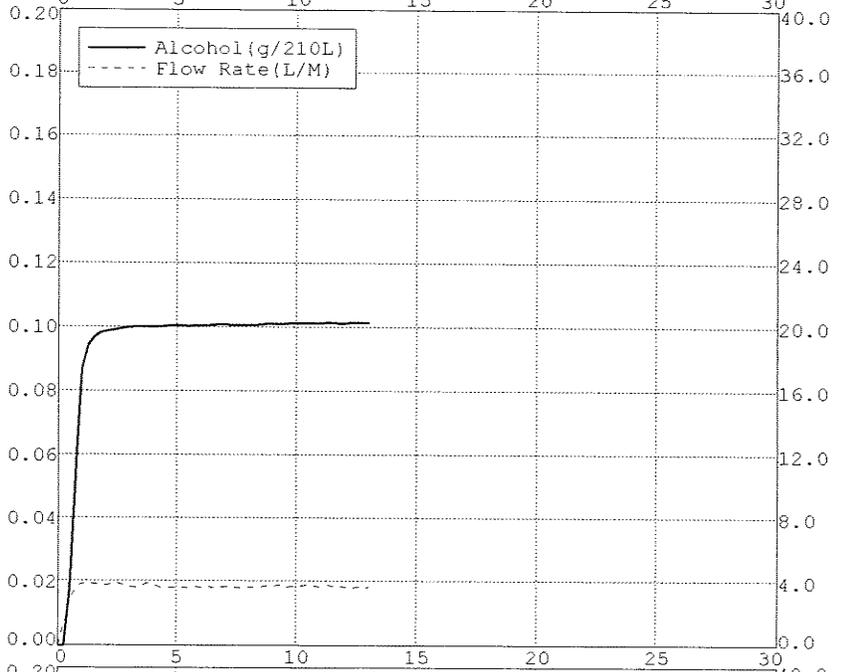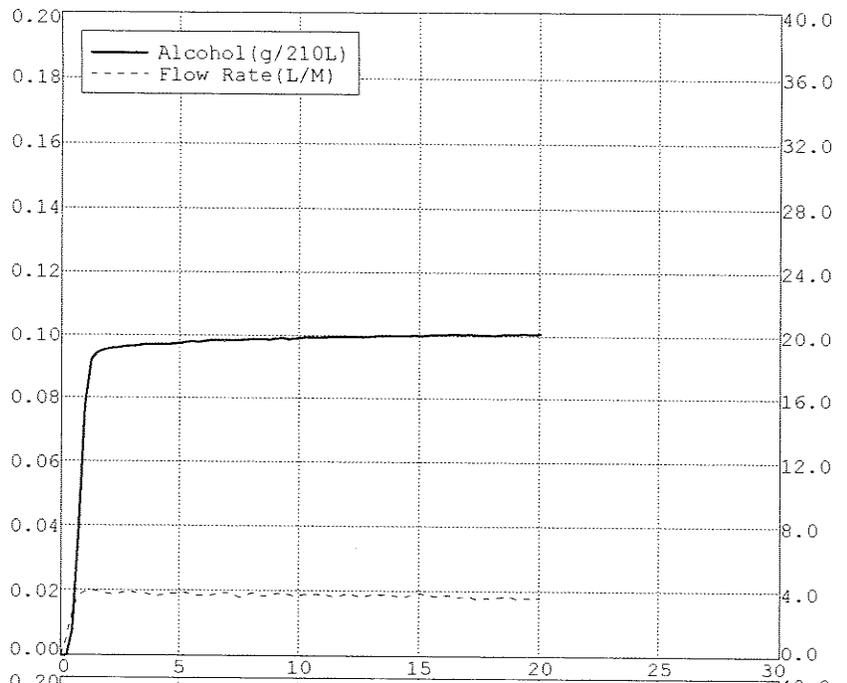

PO Michael Campbell #757