

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/26/2022

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 22100

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:16
INTERNAL STANDARD	VERIFIED	16:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:17
BLANK TEST	0.00	16:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:18
BLANK TEST	0.00	16:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:19
BLANK TEST	0.00	16:20

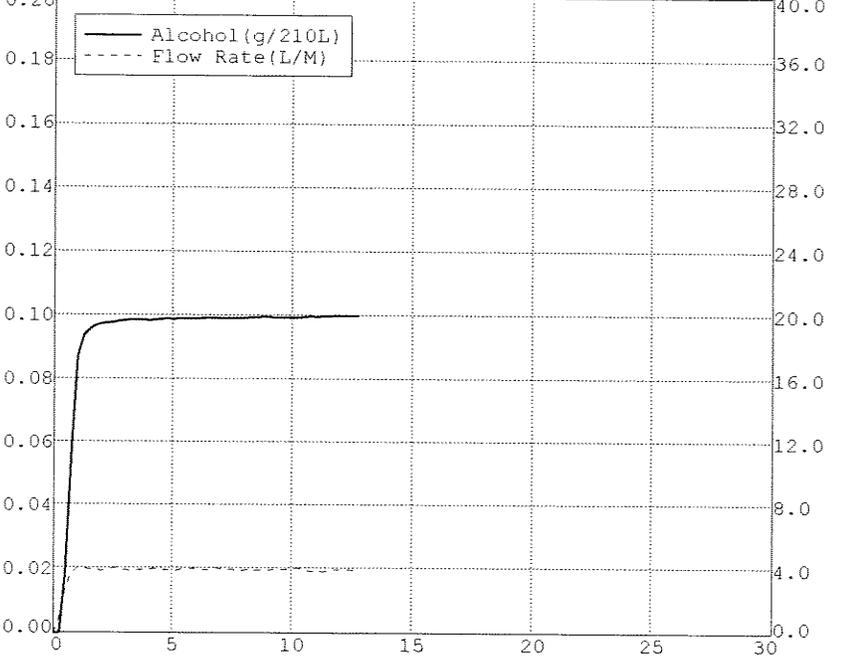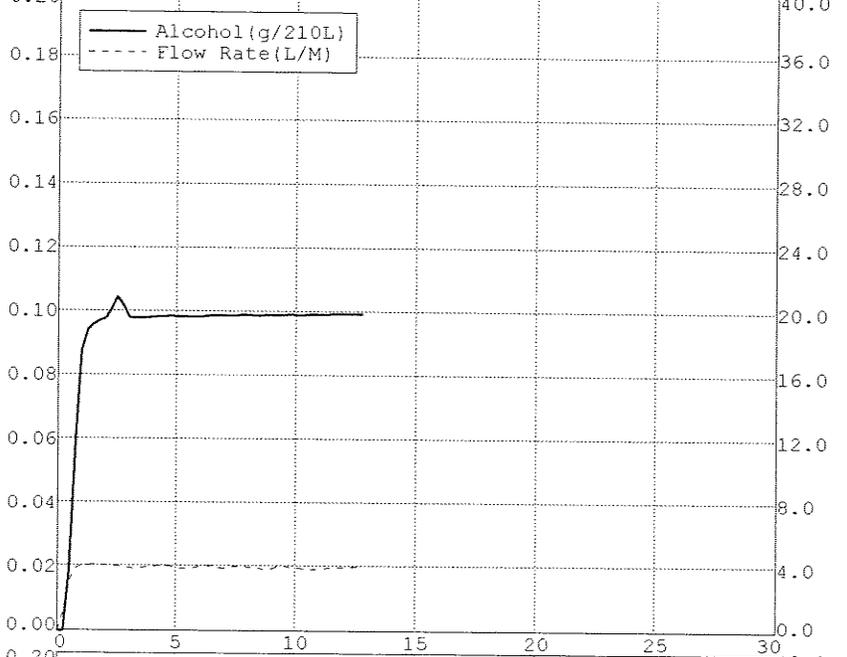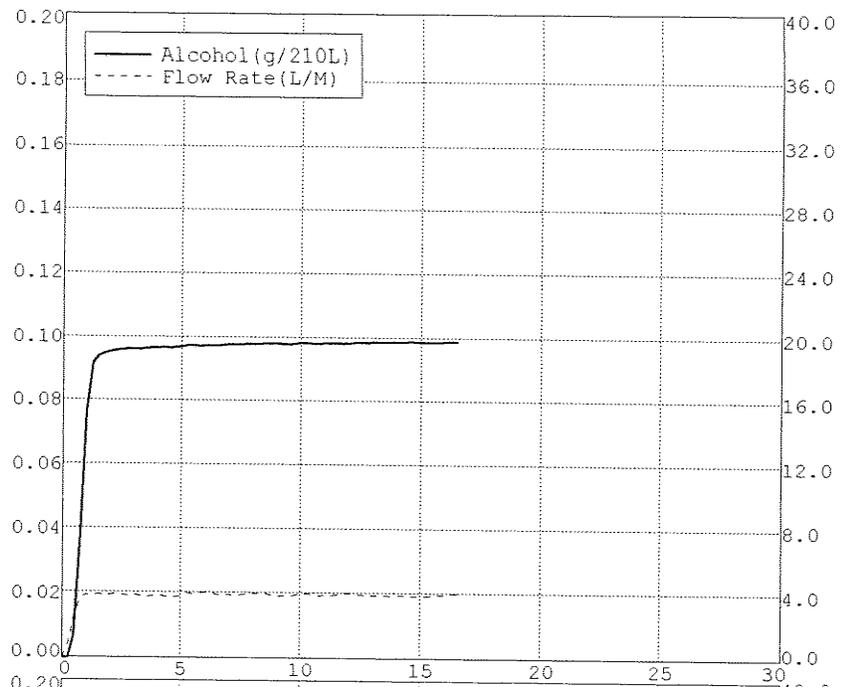

Charles B. Geisler #241