

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 07/31/2022

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 22190

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:06
INTERNAL STANDARD	VERIFIED	11:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:06
BLANK TEST	0.00	11:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:07
BLANK TEST	0.00	11:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:09
BLANK TEST	0.00	11:09

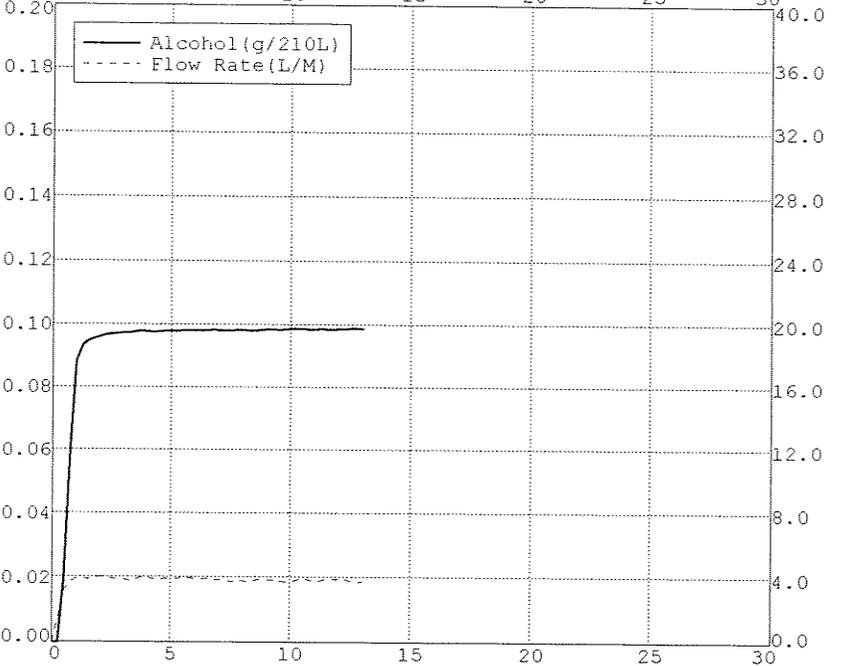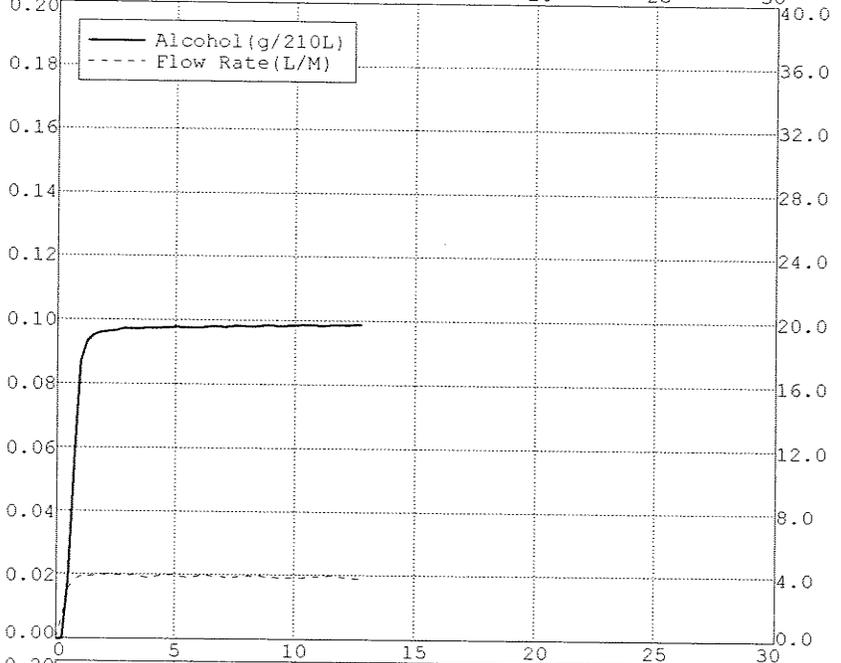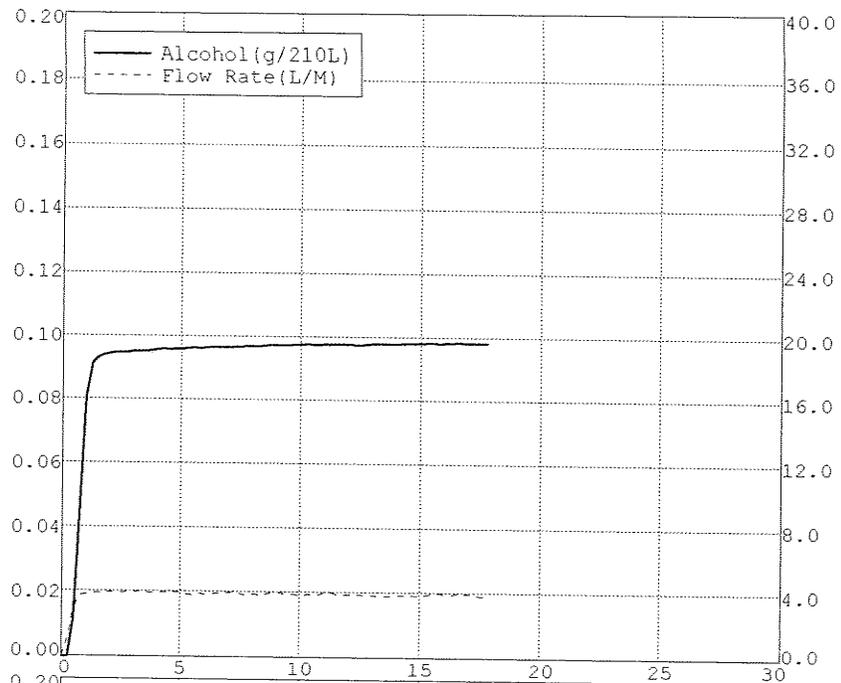

*Handwritten signature and initials* #246